



User's Manual

Purifier® Cell *Logic+* Biological Safety Cabinets

Models

32239 Series	33239 Series	34239 Series
32249 Series	33249 Series	34249 Series
32259 Series	33259 Series	34259 Series
32269 Series	33269 Series	34269 Series

To receive important product updates,
complete your product registration card
online at **register.labconco.com**



*Protecting your
laboratory environment*

LABCONCO®

Labconco Corporation
8811 Prospect Avenue
Kansas City, MO 64132-2696
800-821-5525, 816-333-8811
FAX 816-363-0130
E-MAIL labconco@labconco.com
HOME PAGE www.labconco.com

TYPE

A2

Please read the User's Manual before operating the equipment.

This page is intentionally blank.

Copyright © 2013 Labconco Corporation. All rights reserved.

The information contained in this manual and the accompanying products are copyrighted and all rights reserved by Labconco Corporation. Labconco Corporation reserves the right to make periodic design changes without obligation to notify any person or entity of such change.

Warranty

Labconco provides a warranty on all parts and factory workmanship. The warranty includes areas of defective material and workmanship, provided such defect results from normal and proper use of the equipment.

The warranty for all Labconco products will expire one year from date of installation or two years from date of shipment from Labconco, whichever is sooner, except the following;

- Purifier® Logic®+ Biological Safety Cabinets and PuriCare® Procedure Stations carry a five-year warranty from date of installation or six years from date of shipment from Labconco, whichever is sooner.
- SteamScrubber® & FlaskScrubber® Glassware Washers carry a two-year warranty from date of installation or three years from date of shipment from Labconco, whichever is sooner.
- Blood Drawing Chairs carry a ten-year warranty.
- Carts carry a lifetime warranty.
- Glassware is not warranted from breakage when dropped or mishandled.

This limited warranty covers parts and labor, but not transportation and insurance charges. In the event of a warranty claim, contact Labconco Corporation or the dealer who sold you the product. If the cause is determined to be a manufacturing fault, the dealer or Labconco Corporation will repair or replace all defective parts to restore the unit to operation. Under no circumstances shall Labconco Corporation be liable for indirect, consequential, or special damages of any kind. This statement may be altered by a specific published amendment. No individual has authorization to alter the provisions of this warranty policy or its amendments. Lamps and filters are not covered by this warranty. Damage due to corrosion or accidental breakage is not covered.

Returned or Damaged Goods

Do not return goods without the prior authorization from Labconco. Unauthorized returns will not be accepted. If your shipment was damaged in transit, you must file a claim directly with the freight carrier. Labconco Corporation and its dealers are not responsible for shipping damages.

The United States Interstate Commerce Commission rules require that claims be filed with the delivery carrier within fifteen (15) days of delivery.

Limitation of Liability

The disposal and/or emission of substances used in connection with this equipment may be governed by various federal, state, or local regulations. All users of this equipment are required to become familiar with any regulations that apply in the user's area concerning the dumping of waste materials in or upon water, land, or air and to comply with such regulations. Labconco Corporation is held harmless with respect to user's compliance with such regulations.

Contacting Labconco Corporation

If you have questions that are not addressed in this manual, or if you need technical assistance, contact Labconco's Customer Service Department or Labconco's Product Service Department at 1-800-821-5525 or 1-816-333-8811, between the hours of 7:00 a.m. and 6:00 p.m., Central Standard Time.

TABLE OF CONTENTS

CHAPTER 1: INTRODUCTION	1
CHAPTER 2: PREREQUISITES	2
Space Requirements	2
Clearance	2
Location Requirements	3
Exhaust Requirements	4
Electrical Requirements	4-5
Service Line Requirements	5
User-Supplied Microscope Requirements – With Scope-Ready™ Package Only	6
User-Supplied Microscope Requirements – With Temp Zone™ Package Only	6
CHAPTER 3: GETTING STARTED	7
Unpacking the Biosafety Cabinet	8
Preparing the Biosafety Cabinet for Operation	8
Moving and Lifting the Biosafety Cabinet	9
Installing the Biosafety Cabinet on an Existing Work Surface	9
Installing the Biosafety Cabinet on a Labconco Base Stand	9
Telescoping Base Stands	10
Manual or Electric Hydraulic Lift Base Stands	10
SoLo Electric Hydraulic Lift Base Stands	10
Connecting the Biosafety Cabinet to Utility Service Lines	11
Optional Ventus™ Exhaust System Connections	12
Optional Vacu-Pass™ Cord and Cable Portal Use	13
Drain Valve Installation	14
Microscope Installation (optional)	15-16
Circulator Installation (optional)	17-18
Initial Certification	19

CHAPTER 4: PERFORMANCE FEATURES AND SAFETY	
PRECAUTIONS	20
HEPA Filters	21
ULPA Filters	22
Laminar Airflow	22
Directional Airflow	23
Motor/Blower	24
Cabinet Air Intakes (Grilles), Ductwork & Air Balance Controls	25
Ultraviolet (UV) Lamp	25
Scope-Ready™ Package Option	26
Temp-Zone™ Package Option	26
Safety Precautions	27-28
CHAPTER 5: USING THE CABINET	29
System Reset Switch	29
Information Center	30
Alarm Screens	31
Operating the Sliding Sash	32
Starting the Biosafety Cabinet	32
The Logic+ Touchpad	33
Navigating the Logic+ Menu Screens	34
Navigating the MyLogic™ Menu Screens	35-37
Setting the Clock	35
Configuring the Logic+	36-37
Navigating the Settings Screens	37-40
Units of Measure	37
Security Lock	38
RS-232 Output Rate	38
UV Settings	39-40
UV Lamp Hourmeter	39
Reset UV Lamp Hourmeter	39
Change UV Lamp Life	40
Service Menu Screens	40
Timer Operation	41
Interval Timer Operation	41
Stopwatch Timer Operation	41
If An Airflow Alert Activates	41
Resetting the Airflow Alert System	41
Working in the Biosafety Cabinet	42-44

CHAPTER 6: MAINTAINING THE CABINET	45
Routine Maintenance Schedule	45-46
Service Operations	46-51
Work Surface Removal	46
Front Grille Removal	47
Towel Catch Removal	48
Front Panel Removal & Installation	49
Changing the Fluorescent Lamps	50
Changing the Optional UV Lamp	50
Resetting a Circuit Breaker	51
Storage	51
 CHAPTER 7: TROUBLESHOOTING	 52-54
 APPENDIX A: COMPONENTS	 55-56
 APPENDIX B: DIMENSIONS	 57
 APPENDIX C: SPECIFICATIONS	 58-59
Electrical Data	58
Motor Specifications	58
Environmental Conditions	59
 APPENDIX D: ACCESSORIES	 60
 APPENDIX E: QUICK CHART	 61
 APPENDIX F: INSTALLATION GUIDE FOR ALL PURE-VU SEALS AND STAND-STILL ISOLATION PLATFORMS	 62-70
 DECLARATION OF CONFORMITY	 71



CAUTION – See Manual. When this symbol is on the unit it indicates a caution that is detailed in this manual.

ATTENTION - Voir manuel. Lorsque ce symbole est allumé l'appareil, il indique une mise en garde qui est indiqué dans ce manuel.

Chapter 1: Introduction

Congratulations on the purchase of a Labconco® Purifier Cell Logic+[©] Biosafety Cabinet. The biosafety cabinet is designed to protect you, the product and the laboratory environment from biohazardous aerosols. The Cell Logic Series Cabinet is the result of users like you requiring a customer supplied microscope integrated into the cabinet and a temperature controlled work area to maintain sample temperature. The Cell Logic Biosafety Cabinet is available with either or both Scope-Ready™ and Temp-Zone™ package options.

This biosafety cabinet offers many unique features to enhance safety, performance and ergonomics. To take full advantage of them, please acquaint yourself with this manual and keep it handy for future reference. If you are unfamiliar with how biosafety cabinets operate, please review *Chapter 4: Performance Features and Safety Precautions* before you begin working in the cabinet. Even if you are an experienced biosafety cabinet user, please review *Chapter 5: Using the Cabinet*; it describes the biosafety cabinet's features so that you can use it efficiently.

This manual and other technical information is available in PDF format at our website: www.labconco.com.



If the unit is not operated as specified in this manual it may impair the protection provided by the unit.

Si l'unité n'est pas utilisée comme spécifié dans ce manuel il peut diminuer la protection fournie par l'unité.

Chapter 2: Prerequisites

Before you install the Logic+, you need to prepare the site for installation. Examine the location where you intend to install the cabinet. You must be certain that the area is level and of solid construction. In addition, a dedicated source of electrical power must be located near the installation site.

Carefully read this chapter to learn:

- Location requirements.
- Electrical power requirements.
- Exhaust requirements.
- Service utility requirements.
- Space requirements.
- User-supplied microscope requirements (if needed)
- User-supplied circulator requirements (if needed)

Refer to *Appendix C: Specifications*, for complete biosafety cabinet electrical and environmental conditions, specifications and requirements.

Space Requirements


The dimensions for the Logic+ A2 biosafety cabinets are shown in *Appendix B: Dimensions*.

Clearance

A minimum clearance of at least 6 inches (150 mm) is suggested on the top and both sides of the cabinet for service.

Location Requirements

Note: The biosafety cabinet should be located away from traffic patterns, doors, fans, ventilation registers, fume hoods and any other air-handling devices that could disrupt its airflow patterns. All windows in the room should remain closed. Figure 2-1 shows the preferred location for the biosafety cabinet.

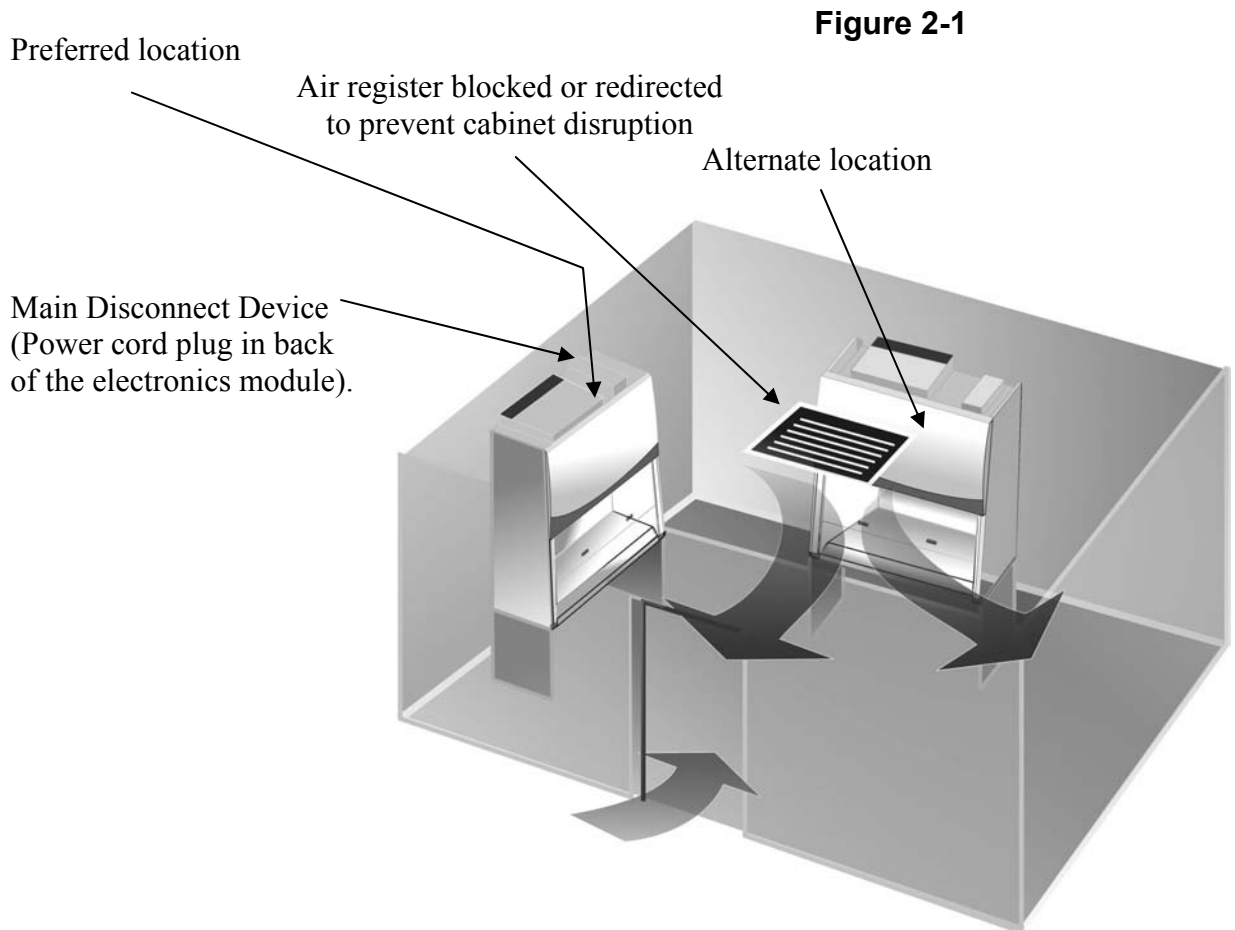

Do not position the unit so that it is difficult to operate the main disconnect device.

Ne placez pas l'appareil de sorte qu'il est difficile de faire fonctionner le dispositif principal de déconnexion.

Exhaust Requirements

If you intend to connect the biosafety cabinet to the optional Ventus™ Canopy Connection Kit, first examine the location to ensure that it accommodates the cabinet's exhaust duct. The area directly above the cabinet's exhaust port should be clear of structural elements, water and utility lines, or other fixed obstructions. There should be enough clearance to accommodate a 10-inch diameter duct. Avoid cabinet locations that require an elbow directly above the cabinet's exhaust connection or an excessive number of elbows in the exhaust system. For further information about the cabinet's exhaust system requirements, please refer to *Chapter 3: Getting Started*.

Electrical Requirements

The biosafety cabinet models have the following electrical requirements:

Table 2-1

Model #	Requirements
3x23xxx0x	115 VAC, 60 Hz, 12 Amps
3x23xxx1x	100 VAC, 50/60 Hz, 12 Amps
3x23xxx-20, 30, 40, 50, 60, 70	230 VAC, 50/60 Hz, 6 Amps
3x24xxx0x	115 VAC, 60 Hz, 12 Amps
3x24xxx1x	100 VAC, 50/60 Hz, 12 Amps
3x24xxx-20, 30, 40, 50, 60, 70	230 VAC, 50/60 Hz, 6 Amps
3x25xxx0x	115 VAC, 60 Hz, 16 Amps
3x25xxx1x	100 VAC, 50/60 Hz, 16 Amps
3x25xxx-20, 30, 40, 50, 60, 70	230 VAC, 50/60 Hz, 8 Amps
3x26xxx0x	115 VAC, 60 Hz, 16 Amps
3x26xxx1x	100 VAC, 50/60 Hz, 16 Amps
3x26xxx-20, 30, 40, 50, 60, 70	230 VAC, 50/60 Hz, 8 Amps

Note: A dedicated outlet with an appropriate circuit breaker should be located as close as possible to the right rear side of the cabinet, at a height even with, or higher than, the top of the bench or stand. Consult your local electrical codes for properly rated circuit breakers. For safe operation the dedicated outlet must provide the protective earthing ground connection to the cabinet.

Note: On 100 and 115 VAC models, both electrical outlets are protected by a ground fault interrupter circuit (GFI). Labconco does not recommend plugging the biosafety cabinet into a GFI outlet.



Electrical outlets in the cabinet are restricted to 5 amps maximum current.

Prises électriques dans l'armoire sont limitées à 5 courant maximum ampères.



Do not use any detachable power cord that is not adequately rated for the unit.

Ne pas utiliser un fil électrique amovible qui n'est pas du tension nominale de l'appareil.

Service Line Requirements

All utility service lines should be ¼ inch O.D., brass, copper, or stainless steel, and equipped with an easily accessible shut-off valve. If the service line pressure exceeds 40 PSI, it must be equipped with a pressure regulator to reduce the line pressure.

Note: The use of flammable gases or solvents should be avoided in the biosafety cabinet. Open flame in the cabinet will disrupt the laminar airflow in the cabinet and may damage the HEPA filters. Flammable gases or solvents may reach explosive concentrations in the cabinet or ductwork. If you feel that the procedure requires the use of an open flame or flammable materials, contact the institution's safety office.

The use of air or gases under high pressure should be avoided as they may seriously disrupt the airflow patterns in the cabinet.

User-Supplied Microscope Requirements – Purifier Cell Logic Biosafety Cabinets with Scope-Ready™ Package Only

If installing a microscope, locate the Stand-Still™ Isolation Platform in a separate box shipped with the cabinet. The Stand-Still Isolation Platform supports the microscope on top of the stainless steel work surface to eliminate up to 94% of vibrations and to promote safe airflow. If using a stereoscope with a forward extending base, the extended Stand-Still XL Isolation Platform should be ordered from *Appendix D: Accessories*. Figures from *Appendix F* should be used to assist your set-up.

On models with the Scope-Ready package, the Cell Logic Biosafety Cabinet includes a clear, disposable Pure-Vu™ Seal that can be altered to accommodate most microscope's eyepieces. Utilize the Punch Kit (#4027801), supplied with your cabinet, to cut the two eyepiece holes at approximately 2.75" (69.9 mm) spacing to match the height of your scope. As a convenience, pre-cut Pure-Vu eyepiece seals can be ordered from *Appendix D: Accessories*. The pre-cut accessory Pure-Vu Seals are based off the nominal height from the base of the microscope to eyepiece centerline and can save you valuable time modifying the seal shipped with the Cell Logic. If using a stereoscope with a forward extending base, one of the Pure-Vu XL Seals should be ordered from *Appendix D: Accessories*. Figures from *Appendix F* should be used to assist your set-up for all Pure-Vu Seals.

User Supplied Circulator Requirements – Purifier Cell Logic Biosafety Cabinets with Temp Zone™ Package Only

The Temp Zone™ features a temperature controlled area on the work surface where heated or chilled samples may be transferred and kept at optimum temperature. A user-supplied circulator that continually delivers heated or chilled water at a minimum flow rate of 0.5 GPM (1.9 LPM) with typical volume of 6 liters is required and may be obtained from your laboratory supply dealer. See Figure 3-6 in *Chapter 3*.

Quick connection fittings are included on the left side of the cabinet and are sized for 3/8" diameter polyethylene tubing. As a convenience, an ample supply (20'; 6 m) of 3/8" (9.5 mm) diameter tubing, insulation, and quick connect fittings (3/8 tube x 1/8 NPT, 3/8 tube x 1/4 NPT, 3/8 tube x 3/8 NPT) are supplied with the Temp-Zone package for connection to a water circulator. The water circulator can be located underneath the work surface of the cabinet or next to the cabinet on the floor.

Chapter 3: Getting Started

Now that the installation is properly prepared, you are ready to inspect, install, and certify the Logic+ biosafety cabinet. This chapter covers how to:

- Unpack and move the biosafety cabinet.
- Install the cabinet.
- Connect the electrical supply source.
- Connect the service lines.
- Connect to an exhaust system (optional).
- Arrange certification of the biosafety cabinet.
- Install the microscope (optional – Scope-Ready package only).
- Connect the circulator (optional – Temp-Zone package only).

Tools required for installation the biosafety cabinet include two 1/2" wrenches, a flat-blade screwdriver, a #2 Phillips screwdriver, and a carpenter's level.

Note: The biosafety cabinet models weigh between 400–700 lbs. (182-318 kg). The shipping pallet allows for lifting with a mechanical lift truck or floor jack. If you must lift the product manually, use at least six (6) persons and follow safe-lifting guidelines.

Unpacking the Biosafety Cabinet

Carefully remove the outer carton and inspect the cabinet for damage that may have occurred in transit. If the biosafety cabinet is damaged, notify the delivery carrier immediately and retain the entire shipment intact for inspection by the carrier.

Note: United States Interstate Commerce Commission rules require that claims be filed with the delivery carrier within fifteen (15) days of delivery.

Do not return goods without the prior authorization of Labconco. Unauthorized returns will not be accepted.

If the cabinet was damaged in transit, you must file a claim directly with the freight carrier. Labconco Corporation and its dealers are not responsible for shipping damages.

Do not discard the carton or packing material for the biosafety cabinet until all of the components have been checked, installed and tested.

The cabinet is secured to the pallet in two places on each side. To access the nuts and bolts, remove the side panels by removing and keeping the two Phillips screws on both panels. Swing the front of each panel away from the cabinet, and lift it straight up to remove the panel from the cabinet.

Note: The side panels must be removed to access the fasteners that secure the biosafety cabinet to the pallet. **DO NOT ATTEMPT TO LIFT THE BIOSAFETY CABINET BY THE SIDE PANELS; DAMAGE WILL OCCUR.**

Preparing the Biosafety Cabinet for Operation

Installation instructions (Labconco P/N 1056801) are attached to the sash of the biosafety cabinet. If these instructions are missing or unclear, contact Product Service at 800-821-5525 or 816-333-8811. The following are located in a box underneath the work surface:

- User's Manual CD
- Drain Valve Assembly and fasteners
- Power Cord
- Product Registration Card
- Vacu-PassTM Accessories (optional)

If you did not receive one or more of the components listed for the cabinet, or if any of the components are damaged, contact Labconco Corporation immediately for further instructions.

Moving and Lifting the Cabinet

Move the cabinet, attached to its pallet, by using a floor jack, or a furniture dolly underneath the unit. **DO NOT** move the cabinet by tilting it onto a hand truck.

When lifting the cabinet **DO NOT** lift the cabinet in the middle front area of the hull. Lifting here may bend or distort the bottom of the cabinet, causing damage to the unit.



Installing the Biosafety Cabinet on an Existing Work Surface

Note: The biosafety cabinet is very top heavy. Use caution when lifting or moving it.

When installing the biosafety cabinet onto an existing work surface or benchtop, ensure that the structure can safely support the combined weight of the cabinet and any related equipment. The work surface should be at least as wide as the cabinet and 31 inches (787 mm) deep to properly support the unit.

A hole or notch may be cut in the supporting surface in the right front corner to accommodate the optional drain valve.

Installing the Cabinet on a Labconco Base Stand

Labconco offers accessory Base Stands in a variety of configurations to suit your particular needs. Stands can be ordered with adjustable telescoping legs or with a manually or electrically adjustable hydraulic lift.

Telescoping Base Stands

These stands are included with some Logic+ models, or are available separately. The base stands for each width cabinet are listed in Table 3-1 below. An optional caster wheel kit is available (part # 3730500).

Table 3-1

Width	Base Stand w/Feet Model #
3'	3401003
4'	3401004
5'	3401005
6'	3401006

Manual or Electric Hydraulic Lift Base Stands

These base stands offer infinitely adjustable height between 25.5 and 33.5 inches (648 to 851 mm), giving a cabinet work surface height of 28.0 to 36.0 inches. The height is adjusted either by a manual (hand crank) or electric pump that drives hydraulic rams in the legs of the stands. All of the hydraulic stands are equipped with fixed feet, but can be converted to caster wheels with the addition of Caster Kit #3784000. The base stands for each cabinet size is listed in Table 3-2 below.

Table 3-2

Width	Manual Lift Stand #	Electric (115V) Lift Stand #	Electric (230V) Lift Stand #
3'	3780200	3780100	3780103
4'	3780201	3780101	3780104
5'	3780203	3780106	3780107
6'	3780202	3780102	3780105

Note: When installing the cabinet on the hydraulic lift base stand, ensure that the hydraulic lines and the electrical cord are clear of any obstructions before installing the cabinet on the stand or operating the lift system.

SoLo™ Electric Hydraulic Lift Base Stands

These base stands permit the Logic+ to be lowered enough to be transferred through a standard doorway as low as 78 inches. Casters provide mobility and lock in place. The SoLo Stands for each Purifier Logic+ series model is listed below.

	115V SoLo Stand #	230V SoLo No. America Plug #	230V SoLo UK Plug #	230V SoLo Schuko Plug #	230V SoLo China/Australia Plug #
3'	3780310	3780314	3780330	3780334	3780338
4'	3780311	3780315	3780331	3780335	3780339
5'	3780312	3780316	3780332	3780336	3780340
6'	3780313	3780317	3780333	3780337	3780341

Connecting the Biosafety Cabinet to Utility Service Lines

Note: Some models have a solenoid valve connected to the service valve on the right side, rear position. The solenoid prevents gas from flowing to the service valve when the unit blower is off. It is the only service valve position that can be fitted with a solenoid valve. Connect the gas service to the solenoid valve.


The service lines (if any) should be connected to the tube fitting(s) on the outside of the liner wall as shown in Figure 3-1. To install the tubing, follow these steps:

1. Ensure that the tubing is $\frac{1}{4}$ inch O.D., soft metal, and that the end has been completely deburred.
2. Route the tubing from the rear of the cabinet, ensuring that it will line up with the slot in the back of the side panel. The slot is located from $8\frac{3}{4}$ to $11\frac{1}{4}$ inches (222 to 288 mm) from the bottom of the cabinet.

Note: Make sure that the tube routing will not contact any electrical wires. DO NOT loop service line tubing within the side panels of the cabinet.

3. Make sure that the nut on the tube fitting is loose, but do not remove it. Look inside the fitting to make sure the tube ferrule is there.
4. Push the tube into the fitting until it is properly seated. The tube will go approximately $\frac{3}{4}$ inch (19 mm) into the fitting.
5. Tighten the tube fitting nut hand tight and then, using a $\frac{7}{16}$ -inch wrench, tighten it at least $\frac{3}{4}$ turn more.
6. Close the service valve in the biosafety cabinet and then slowly open the shutoff valve on the service valve. Test all fittings for leakage. Tighten the tube nut slightly if needed.

Figure 3-1

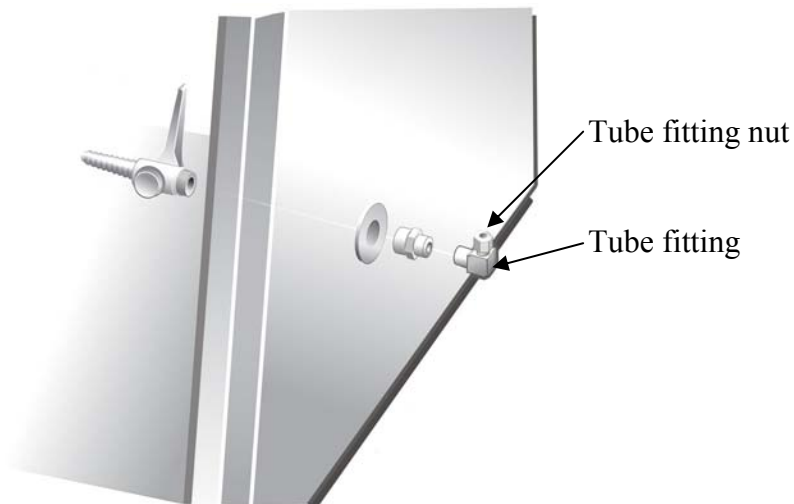

Optional Ventus™ Canopy Exhaust Connection

Certain applications such as working with odorous products or volatile toxic materials will require the connection of the biosafety cabinet to an exhaust system.

Note: The canopy connection, also referred to as a thimble or air gap connection, allows single or multiple biohazard cabinets to be connected to an exhaust system. During operation, the exhaust system draws all of the cabinet's exhaust air, plus a volume of room air (through the vent in the canopy) into the exhaust duct. Canopy connections function as a "shock absorber" allowing the system to function properly during changes in room air pressure.

For information on selecting a canopy connection, go to *Appendix D: Accessories*.

Note: If the research involves the use of toxic compounds or volatile materials, contact the facility's safety officer or Labconco to ensure that the biosafety cabinet and its exhaust system are compatible with the materials you will be working with.

Optional Vacu-Pass™ Cord & Cable Portal Use

Note: There must be enough clearance to pass the cord or cable between the Logic+'s exterior dress panel and any obstruction.

Note: Some Vacu-Pass components and the cord or cable passing through it may become contaminated during use of the cabinet. Ensure all potentially contaminated components are surface decontaminated before handling or removal from the cabinet.

1. Remove the grommet from the liner side wall. Remove the solid sealing plug from the body of the portal by either pressing it through from the outside, or by carefully inserting a spatula or similar device between the sealing plug and the body of the portal, and prying the plug out.
2. Pass the cord or cable through the body of the portal, and then through one of the plugs that has been cut for cord or cable use, then through the grommet, as shown in Figure 3-2.

Note: select a plug with a hole that is slightly smaller than the cord or cable, to create a proper seal. This will also help minimize movement of the cord or cable if it is accidentally pulled during use.

Figure 3-2



3. Position the cord or cable as it will be used in the cabinet, and then push the plug back into the body of the portal until it seats in the portal. Reinstall the grommet.

Drain Valve Installation

In order to prevent damage during shipping, the drain valve assembly has not been installed. If desired, the valve should be installed after the cabinet is in its final location.

To install the valve assembly, follow these steps:


Note: The work surface is heavy. Use caution when handling it.

4. Lift the work surface out of the biosafety cabinet by lifting on the knobs at the front of the work surface. Steady the work surface while pulling it straight out the front of the cabinet.
5. Using a putty knife, remove and discard the stainless steel cover that is sealed over the drain mounting holes. Scrape out remaining sealant that is around the holes.
6. Apply a light coating of silicone sealant (user supplied) to the mounting surface of the drain assembly. Attach the drain assembly under the bottom of the cabinet as shown in Figure 3-3. Wipe off any excess sealant from the cabinet bottom. Ensure that the center drain hole is unobstructed.
7. Make sure the drain valve is in the closed position.
8. Reinstall the work surface.
9. Allow the silicone sealant to cure for at least eight hours before exposing it to liquid.

Figure 3-3

NOTE: The drain valve assembly attaches to the underside of the cabinet bottom.

Apply a light coat of silicone sealant to this surface of the connector, aligning the three holes in the connector with the three holes in the biosafety cabinet liner.

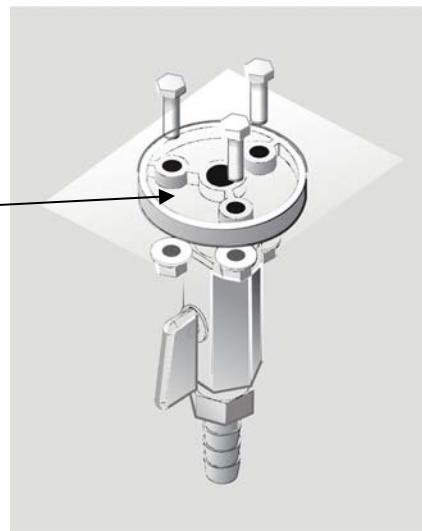

Microscope Installation (optional)

In order to successfully install a user-supplied microscope in a Cell Logic Biosafety Cabinet with Scope-Ready package, please follow the steps below and refer to Figure 3-4 as well as *Appendix F: Installation Guide for all Pure-Vu Seals and Stand-Still Isolation Platforms*:

Note: The work surface is heavy. Use caution when handling it.

1. Before installing a microscope, locate the Stand-Still Isolation Platform that is packaged in a separate carton underneath the work surface. **Note:** Stereoscopes will typically require the Stand-Still XL Isolation Platform found at www.labconco.com.
2. Install the Stand Still Isolation Platform so that the leading edge is in line with the work surface leading edge. The Stand-Still Isolation Platform is elevated to promote safe airflow and isolate up to 94% of vibrations. See *Appendix F* for typical pictures of proper set-up of the Stand-Still Isolation Platform.
3. With the sash in the up position, place a user-supplied microscope inside and on top of the Stand-Still Isolation Platform. Remove the microscope eyepieces.
4. The Cell Logic Biosafety Cabinet with Scope-Ready Package includes one Pure-Vu Seal that requires 0.5" (12.7 mm) diameter holes spaced approximately 2.75" (69.9 mm) apart and located from the base of the microscope to the centerline of the eyepiece. The eyepiece holes can be cut with the 0.5" (12.7 mm) diameter hole Punch Kit (#4027801) supplied with your cabinet.


For your convenience, pre-cut accessory Pure-Vu Seals are available per www.labconco.com, and may be an easier installation.

5. If punching the 0.5" (12.7 mm) diameter holes, remove the microscope eyepieces and line up the centerline of the eyepiece base with the seal. Then mark the centerline of each eyepiece hole spaced at approximately 2.75" (69.9 mm).
6. Remove the 14 screws (#6-32 x 0.25") that retain the Pure-Vu Seal.
7. Either reinstall one of the pre-cut accessory Pure-Vu Seals from *Appendix D* or punch the holes in the blank seal supplied and then re-install the seal. For your convenience, see *Appendix F* for installation of pleated Pure-Vu XL Seals used with stereoscopes requiring frequent eyepiece height adjustment of +/- 2.0" (51 mm).
8. After the seal is re-installed, then move the microscope forward to carefully stretch the Pure-Vu Seal over both of the microscope eyepiece bases.

Chapter 3: Getting Started

9. Finally, re-install the microscope eyepieces.
10. The Pure-Vu Seal should now provide an optimum seal for safe airflow and ergonomic visibility.

Figure 3-4

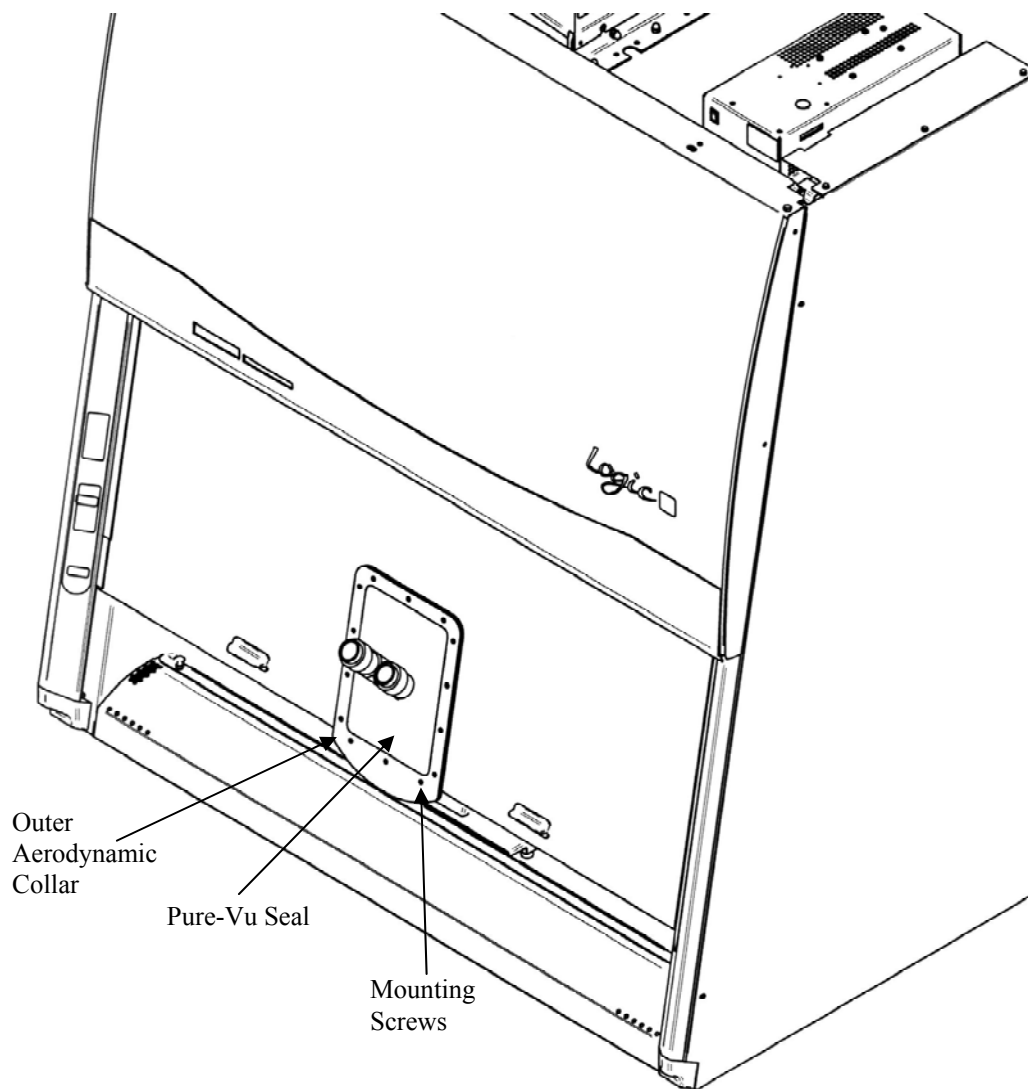

Circulator Installation (optional)

In order to successfully install a user-supplied circulator on a Cell Logic Biosafety Cabinet with Temp-Zone package please follow the steps below and refer to Figure 3-5:


Note: The work surface is heavy and two Easy-Clean™ Prop Rods are provided to pivot and support the Temp-Zone work area and the work surface.

1. The Temp-Zone work area has supply and return lines for the user-supplied circulator. Refer to Figure 3-5 and locate the two quick connect elbows on the left side of the cabinet behind the left side panel.
2. Find a suitable place next to the cabinet or underneath the cabinet to place the circulator. Accessory shelves for small circulators are available from www.labconco.com. Larger circulators should be placed on the floor.
3. Pivot the work surface up and use the Easy-Clean Prop Rods to support the work surface. Then locate the tubing, insulation, and quick connect fittings shipped with your Cell Logic. The tubing is 3/8" OD (9.5 mm) and tube inserts must be placed inside the tubing to properly support the tubing inside the quick connect fitting. 20 feet (6.1 meters) of tubing length is provided for your convenience.
Note: The tube inserts prevent the tubing from collapsing at connection points and must be used.
4. Plan, route and cut the tubing from the two elbows on the left side of the cabinet to the circulator.
5. Locate the quick connect fittings (3/8" tube x 1/8 NPT, 3/8" tube x 1/4 NPT, and 3/8" tube x 3/8 NPT) and install the appropriate fittings to the user-supplied circulator with appropriate pipe sealant or PTFE tape.
6. Place tube inserts in all ends of the cut-to-size tubing.
7. Cut and install the insulation around the cut tubing lengths.
8. Insert cut tubing lengths into the elbows on the cabinet and then install both tubing lengths into the circulator to complete the water circulator loop.
9. Read and follow the circulator instructions before operating. The circulator should have a minimum flow rate of 0.5 GPM (1.9 LPM). In all cases, the temperature of the circulator will not equal the temperature of samples on the Temp-Zone. Factors such as the sample vessels, sample sizes, aluminum tube racks, and length of tubing connecting the circulator to the Temp-Zone can influence the sample temperature. Circulator settings to hold heated incubator sample temperatures may require 0.3-2.0°C higher temperatures than the desired sample temperature. Furthermore, circulator settings to maintain chilled refrigerated samples may require 0.3-3.0°C colder temperatures than the desired sample temperature. Experimentation is necessary to achieve proper sample temperatures.

Chapter 3: Getting Started

10. For chilled applications, the Temp-Zone work area comes with a drain line installed that can be routed to the cabinet's drain valve, if desired. This Temp-Zone drain line installation is optional for chilled applications should excessive condensation occur under the work surface. Simply snap in the supplied press-fit elbow to the drain valve shown in Figure 3-5. Follow the diagram to finish the installation.

Figure 3-5

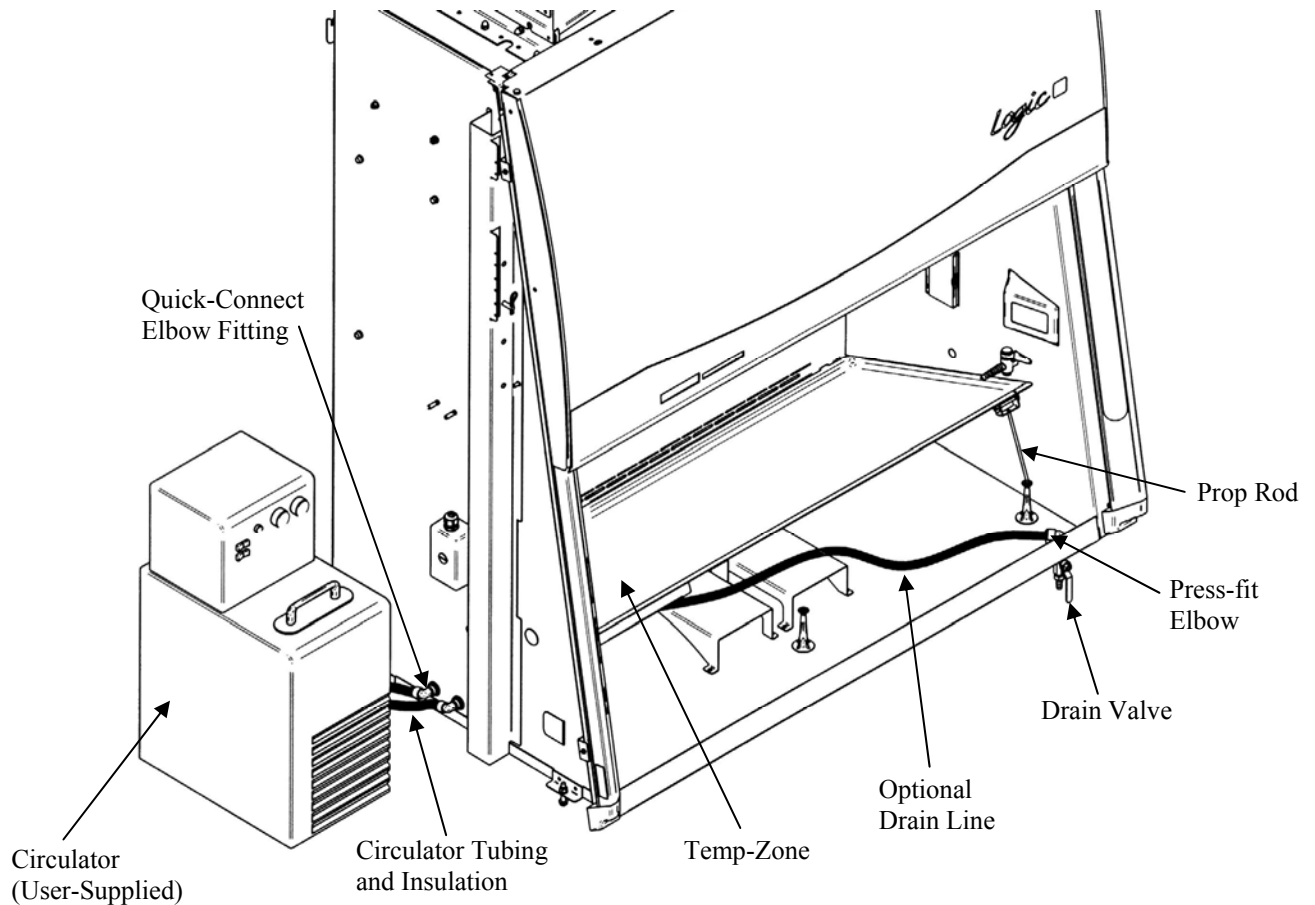

Initial Certification

Prior to use, a qualified certifier should certify all biosafety cabinets. Under normal operating conditions, the biosafety cabinet should be recertified at least annually and when relocated or serviced. The certifier should perform the following tests, as recommended in ANSI/NSF International Standard Number 49 in effect when the cabinet was manufactured:

- Downflow Velocity Profile Test
- Inflow Velocity Test
- Airflow Smoke Patterns
- HEPA Filter Leak Test
- Optional Canopy Alarm Test and Operation
- Vibration Test *
- Noise Level Test *
- Lighting Intensity Test *

*These tests are user comfort related tests and may be omitted at the user's or certifier's discretion.

If you have any questions regarding certification agencies or need assistance in locating one, contact Labconco's Product Service Department at 1-800-522-7658 or 816-333-8811.

Chapter 4: Performance Features and Safety Precautions

All Purifier Logic+ Biosafety Cabinets operate using the following principles:

- Filtration and retention of particulates by High Efficiency Particulate Air (HEPA) filter(s)
- Laminar airflow
- Directional airflow

The major components in a biosafety cabinet are:

- The HEPA filter(s) or optional ULPA filters
- The motor/blower to force air through the cabinet
- Cabinet air intakes (grilles), ductwork and air balance controls

The two major package options of a Cell Logic Biosafety Cabinet are:

- The Scope-Ready™ package option to allow a user-supplied microscope to be integrated into the cabinet.
- The Temp-Zone™ package option that includes a temperature controlled work area when connected to a user-supplied circulator.

HEPA Filters


HEPA filters are disposable, dry-type particulate filters. The filter material or media is typically made of borosilicate microfibers formed into a thin sheet, in a process similar to the production of paper. This sheet is folded, or pleated to increase its surface area. The pleats are typically held in place by beads of glue that add rigidity to the media pack. The pack is then set into a frame, and sealed as shown in Figure 4-1.

The HEPA filter manufacturer establishes the efficiency of the filter by challenging it with an aerosol of known particle size. The number of particles that penetrate the filter are quantified, and this establishes the efficiency of the filter. Thus, the filters used in the Logic+ cabinets are at least 99.99% efficient in removing particles 0.3 micron.

Note: The HEPA filter media is very fragile. DO NOT touch the media. If you think the media of a HEPA filter is damaged, DO NOT USE THE CABINET. Have the HEPA filter integrity tested by a certifier before using the cabinet.

Note: HEPA Filters are only effective against particulate material. Gases will pass through the filter.

Figure 4-1

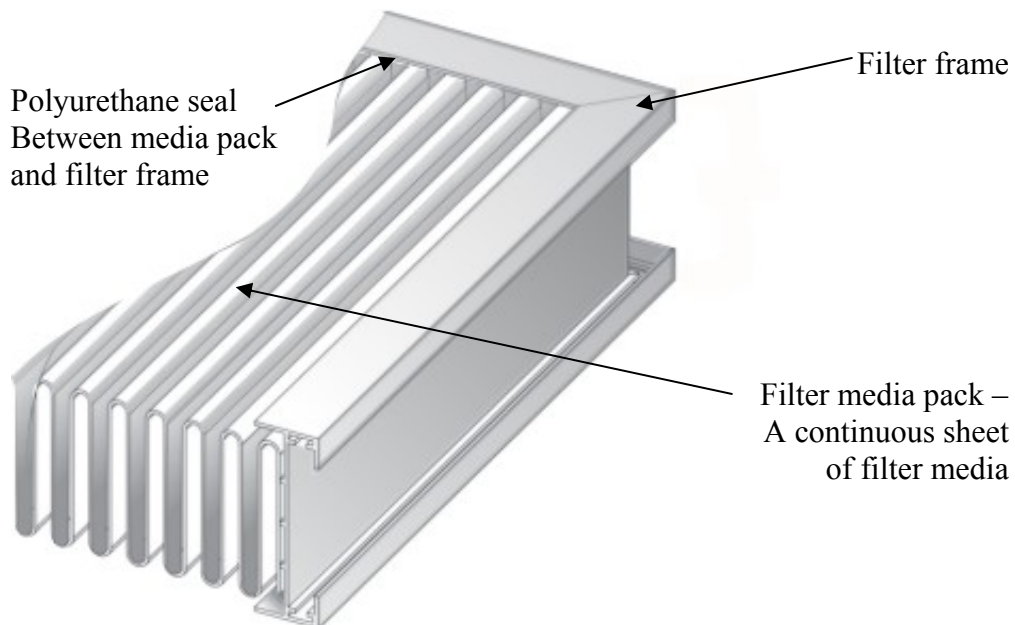

ULPA Filters

Optional ULPA filters may be used to replace the standard HEPA filters in the Purifier Logic+ biosafety cabinets. ULPA filters have the same properties as described above except they are rated at least 99.999% efficient in removing particles 0.1-0.2 or 0.2-0.3 micron.

Laminar Airflow

Laminar airflow is defined as the movement of a body of air in a single direction, with a uniform velocity. In practice, the laminar downflow of air in the cabinet captures any aerosol generated in the work area of the cabinet, and directs it to the HEPA filters. In order to be true laminar downflow, a number of individual downflow velocity test points (The Downflow Velocity Profile) must be ± 16 feet per minute (0.08 m/s) of the average of all the test points. This is illustrated in Figure 4-2.


Figure 4-2



Directional Airflow

Directional airflow also plays a key role in biosafety cabinet performance. Air is drawn into the front of the cabinet at the front grille. This “curtain” of air makes it more difficult for aerosols to escape out of the work area of the cabinet and into the outside environment. This airflow is often calculated and referred to as the **Inflow Volume** or **Average Inflow Velocity**. This is illustrated in Figure 4-3.


Figure 4-3

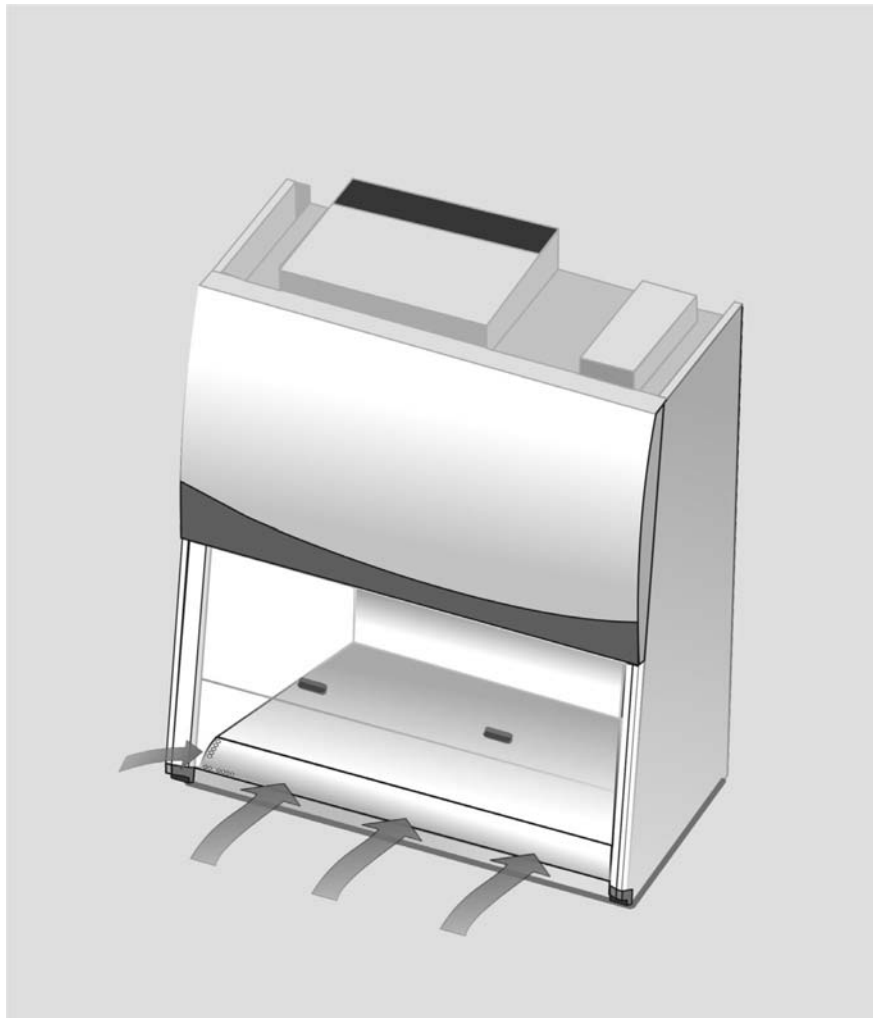

Motor/Blower

The motor/blower assembly pulls room air into the front of the cabinet, and re-circulates it internally. During its recirculation, the air is split into two separate streams. One path leads through the exhaust HEPA filter and out of the unit. The second path flows through the supply HEPA filter, which then flows down through the work area, as shown in Figure 4-4. The motor in the Logic+ cabinet is an electronically commutated motor (ECM). The ECM is a brushless DC motor that includes its own power supply to convert the incoming alternating current to direct current, as well as its own microprocessor to control and measure the motor's operation. The motor utilizes Labconco's exclusive Constant Airflow Profile™ (CAP) program to deliver a consistent volume of air, throughout the life of the cabinet.

Figure 4-4

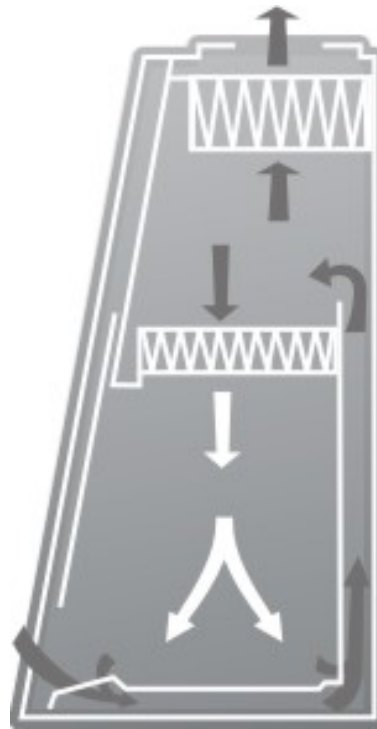

Cabinet Air Intakes (Grilles), Ductwork and Air Balance Controls

The location, size, and pattern of the grilles at the front and rear of the work area affect cabinet containment and performance.

Note: Do not block or obstruct the grilles of the biosafety cabinet.

The internal ductwork of the biosafety cabinet conveys the air from the work area to the blower, and then from the blower to the filters. The positive pressure rigid plenum of the biosafety cabinet is designed to deliver a more uniform airflow to both HEPA filters, optimizing filter loading and operational life.

Ultraviolet (UV) Lamp

The optional UV lamp generates a primary wavelength of light of 254nm. A secondary emission is in the visible (blue) wavelength, resulting in the characteristic blue color while operating. UV light at this wavelength is biocidal, primarily by creating thymine dimers in DNA. These dimers prevent the correct transcription of the DNA into RNA, resulting in cellular death or viral inactivation. In order to be effective, the UV light must directly strike the nucleic acid, and its effectiveness can be diminished or negated by dissolved proteins or metals, or by other UV-opaque substances protecting the target nucleic acid.

Because of its limitations, UV light should be used as an adjunct to good surface disinfection practices. In order to get optimum performance from the UV light, it should be replaced after 6,000 hours of operation or less, and the exterior surface of the lamp should be kept clean and free of dust.

Note: The Logic+ records the number of hours of operation of the UV light. You can program in the number of hours (in 100-hour increments) it will operate before a replacement message is displayed.

Note: UV irradiation is absorbed by the tempered safety glass of the sash. Independent research has shown that the level of UV irradiation on the outside of the cabinet's sash is equal to background radiation levels.

Note: The UV sensitivity of a target organism varies, depending on the UV output of the lamp, the genus and species of the organism, the medium the agent is suspended in, etc. Contact the Health and Safety Officer at your facility for UV light use and recommendations.

Scope-Ready™ Package Option

Models with the Scope-Ready package option allow a user-supplied microscope to be integrated into the safety cabinet. On these models, two features work together to assure containment and reduced vibration:

- The Pure-Vu™ Seal includes a 7" wide x 10.5" (267 mm) high sash cutout that accommodates most microscopes' eyepieces. The clear disposable eyepiece seal prevents contaminants from escaping while providing ergonomic visibility into the cabinet. The easy removable seal attaches tightly to an aerodynamic, epoxy-coated steel collar. The unique teardrop shape of the aerodynamic collar design keeps contaminants contained with the microscope in place. The Pure-Vu Seal conforms to both ASHRAE 110 and NSF 49 testing criteria.
- The Stand-Still™ Isolation Platform supports the microscope on the cabinet's work surface and removes up to 94% of vertical and horizontal vibrations. ASHRAE 110 and NSF 49 testing confirms this unique elevated, aerodynamic base ensures safe airflow. Constructed of seamless Type 304 stainless steel, the isolation platform is non-porous, easy to clean, and autoclavable. **Important Note:** Always remove the rubber isolation feet prior to autoclaving. The spacious 12" (305 mm) wide x 18.75" (476 mm) deep platform fits most microscopes. See *Appendix D: Accessories* for ordering an extended Stand-Still XL Isolation Platform for use with microscope bases that extend over the front of the lower work surface.

Temp-Zone™ Package Option

Models with the Temp-Zone package option include a temperature controlled area 10.5" (267 mm) wide x 12" (305 mm) deep (7" (178 mm) wide x 12" (305 mm) deep on 3' models). Samples heated in an incubator or chilled in a refrigerator may be transferred to the Temp-Zone and kept at optimum temperature. Quick connection fittings on the left side of the cabinet attach to a user-supplied circulator that continually delivers heated or chilled water through channels located underneath the Temp-Zone area of the work surface. Uniform temperature distribution is maintained on the Temp-Zone area of the work surface. Temp-Zone work area temperatures of 0.3-0.5°C are maintained with the circulator heated to 37°C and within 0.3-1.6°C with the circulator chilled to 3.7°C. Actual set points will vary depending on variables such as sample tube rack, sample size, and length of tubing.

Safety Precautions

Note: The biosafety cabinet should be certified by a certification technician before its initial use. The cabinet should be recertified whenever it is relocated, serviced or at least annually thereafter. Filter integrity and airflow performance should be verified before using the cabinet.

Some internal components of the biosafety cabinet may become contaminated during operation of the unit. Only experienced personnel competent in decontamination procedures should decontaminate the cabinet before servicing these components. If you have any questions regarding certification agencies, or need assistance in locating one, contact Labconco's Product Service Department at 800-821-5525 or 816-333-8811.

DO NOT load more than 50 lbs. (23 Kg) in the work area. Exceeding this limit may damage the work surface and its supports. Excessive weight in the cabinet may increase the risk of it overturning, or failure of hydraulic lift stands, resulting in the cabinet and stand overturning. If your application requires loading more than 50 lbs., contact Labconco's Product Service Department at 800-821-5525 or 816-333-8811 for assistance.

Ensure that the cabinet is connected to electrical service in accordance with local and national electrical codes. Failure to do so may create a fire or electrical hazard. Do not remove or service any electrical components without first disconnecting the biosafety cabinet from electrical service.

Avoid the use of flammable gases or solvents in the biosafety cabinet. Care must be taken to ensure against the concentration of flammable or explosive gases or vapors. An open flame should NOT be used in the biosafety cabinet. Open flames will disrupt airflow patterns, burn the HEPA filter and/or damage the filter's adhesive. Gases under high pressure should not be used in the biosafety cabinet, as they may disrupt its airflow patterns.

HEPA filters only remove particulate matter. Operations generating volatile toxic chemicals or radionuclides must be evaluated carefully.

The media of HEPA filters is fragile and should not be touched. Avoid puncturing either HEPA filter during installation or normal operation. If you suspect that a HEPA filter has been damaged, DO NOT use the cabinet; contact a local certification agency or Labconco at 800-821-5525 or 816-333-8811 for re-certification information.

The HEPA filters in the biosafety cabinet will gradually accumulate airborne particulate matter from the room and from work performed in the cabinet. The rate of accumulation will depend upon the cleanliness of the room air, operating time and the nature of work being done in the cabinet. The Filter Gauge accurately displays the amount of filter life remaining.

Chapter 4: Performance Features and Safety Precautions

Proper operation of the cabinet depends largely upon its location and the operator's work habits. Consult the Installation and Normal Operation sections of this manual for further details.

Avoid direct exposure of plastic or coated materials to ultraviolet (UV) radiation. Never bypass the UV safety interlock that only allows the UV light to work when the sash is closed. When surface disinfecting the biosafety cabinet:

- Avoid splashing the disinfecting solution on skin or clothing.
- Ensure adequate ventilation.
- Carefully follow the disinfectant's safety instructions.
- Always dispose of disinfecting solutions in accordance with local and national laws.
- DO NOT allow disinfectants with high concentrations of free chlorine to contact the stainless steel components of the biosafety cabinet for a long period of time. Free chlorine will corrode stainless steel after extended contact.

Biosafety cabinets should be decontaminated for any of the following reasons:

- Before maintenance work requiring entry into contaminated areas.
- Before HEPA filter changes.
- Before performing certification tests requiring entry into contaminated areas.
- Before relocating the cabinet.
- Before changing research programs.
- After the gross spill of biohazardous material or toxic chemicals.


Chapter 5: Using the Cabinet

System Reset Switch

The biosafety cabinet has a system reset switch for resetting its microprocessors. The switch is located on the front of the electronics module, on top of the cabinet, as shown in Figure 5-1. Ensure that the switch is in the “ON” (up) position before attempting to operate the cabinet.

Figure 5-1

The System Reset
Switch

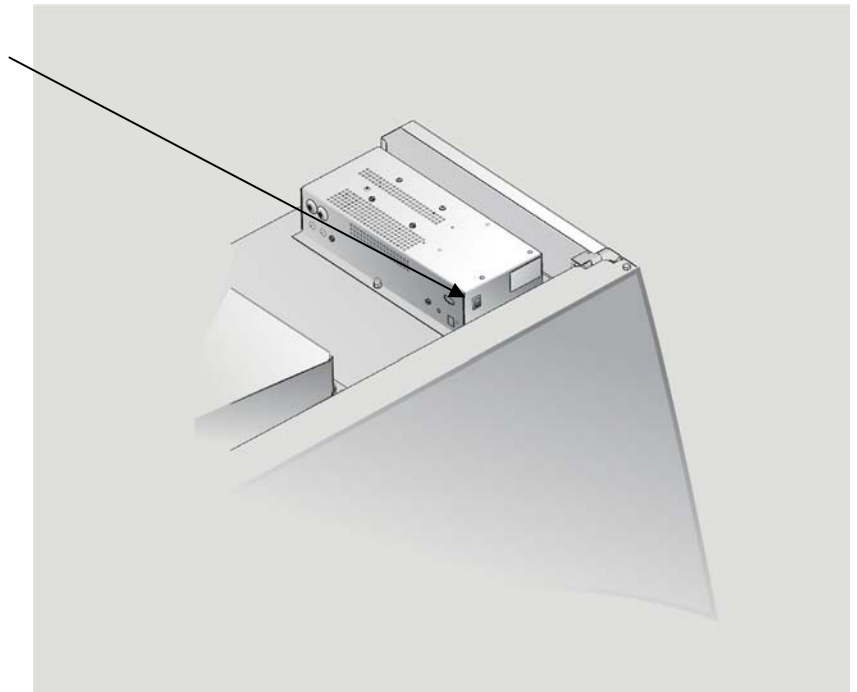

Information Center

The Information Center is an LCD display located on the right side wall at eye level. When the blower is started, the words “please wait” will be displayed, as shown in Figure 5-2. After approximately 90 seconds, the display will switch to normal operation.


The display provides a clock, the remaining filter life, the cabinet’s current status, inflow and downflow velocities (if equipped with the optional airflow sensor), as shown in Figure 5-3. In the event of an alarm, the Information Center will immediately display a context sensitive display indicating the cause of the alarm, and possible solutions, as shown in Figure 5-4.

The display will enter sleep mode, turning itself off, one minute after the blower is turned off or the sash is closed.

Figure 5-2



Figure 5-3

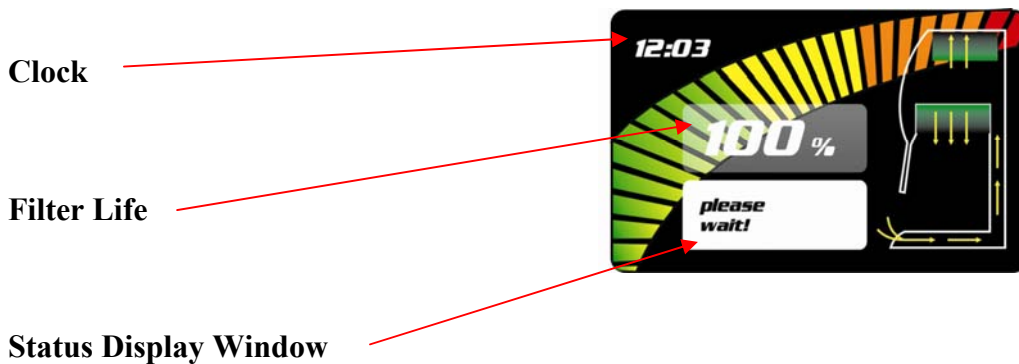

Alarm Screens

Sash is too high

The sash is open too far for safe operation.

Figure 5-4a



Airflow Alert

The airflow patterns in the cabinet have changed, resulting in a sudden change in the motor speed. This is most likely due to a blockage of the grille or the exhaust filter outlet. It may also be caused by removal of the work surface while the cabinet is in operation.


Figure 5-4b



Airflow Alarm

If equipped with the optional airflow sensor and the inflow or downflow velocities are excessively high or low, this alarm will be displayed.


Figure 5-4c

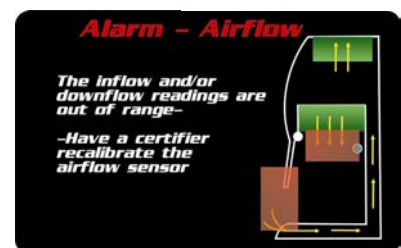

Canopy Alarm

If equipped with the optional canopy connection, and there is insufficient exhaust system airflow, this alarm will be displayed. If this alarm is displayed, the Logic+ blower will need to be turned off, and then back on again to reset the alarm.

Figure 5-4d

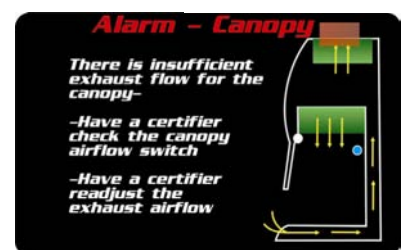

System Error

The motor and display circuit board are not communicating properly. DO NOT USE THE CABINET UNTIL THE PROBLEM HAS BEEN CORRECTED.

Figure 5-4e



Operating the Sliding Sash

The counterbalanced, anti-racking sash mechanism requires only a few pounds of force to move the sash up or down. You can open or close the sash smoothly with one or two hands positioned on either handle.


The sash position alarm and safety interlock system senses the sash position and acts appropriately. The biosafety cabinet has been programmed to operate at either an 8- or 10-inch (203-254 mm) sash opening, depending on model. Raising the sash above its operating height will activate the audible and visual alarms. The audible alarm can be temporarily muted (for approximately five minutes) by depressing and releasing the **OK/Mute** button. Closing the sash back to its operating position will reset the alarm and defeat the muting of the alarm. The safety interlock system senses when the sash is closed and allows the optional ultraviolet (UV) lamp to operate only when the sash is closed, to protect the operator from irradiation.

Starting the Biosafety Cabinet

1. To start the biosafety cabinet, raise the sash until its bottom edge aligns with the sash position label on the left corner post. The decal is shown in Figure 5-5.
2. Press the blower button to start the unit. The unit will display a standby screen for approximately 90 seconds to allow the cabinet to reach proper operating conditions. If the alarm sounds, recheck the sash position. If the sash is too high, the sash audible alarm and the LCD display will indicate the sash is too high.
3. To turn the UV light on, the sash must be completely closed to prevent the escape of any UV radiation. Push the UV light button to activate the UV light.

Note: The sash must be completely closed for the UV light to activate.

Figure 5-5

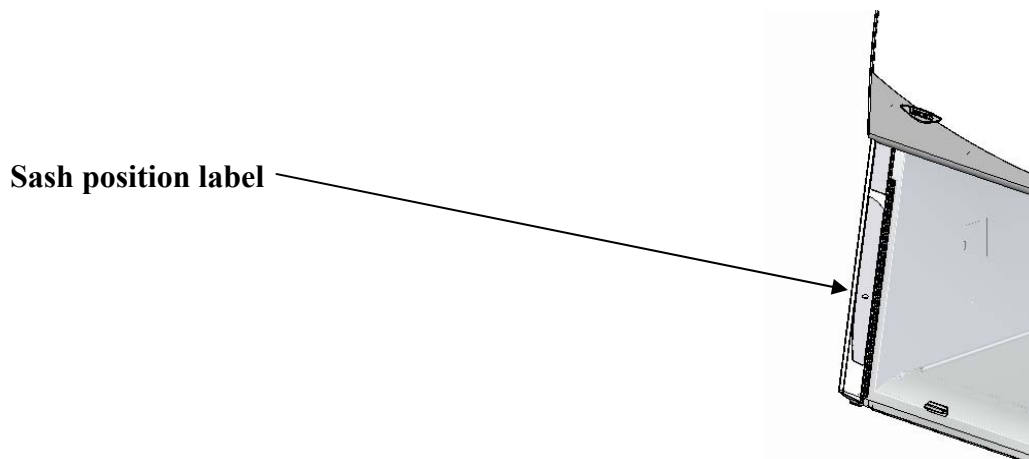

The Logic+ Touchpad

The touchpad of the Logic+ is shown in Figure 5-6. Take a moment to get familiar with the buttons, their locations and functions. Also familiarize yourself with the display located on the right side wall. The display will report system functions, such as filter capacity, timer displays, alarm or error messages, as well as icons that illuminate when cabinet functions such as UV light and blower are operational.

Figure 5-6

Blower Button – Starts or stops the cabinet blower. When the blower is in Smart-Start™ mode, opening the sash from the closed position turns the blower on automatically. In Night-Smart™ mode, when the sash is closed, the motor slows to idle to maintain air cleanliness in the work area. When the sash is reopened, the blower resumes normal operation. Pressing this button overrides Smart-Start and Night-Smart operation.

Light Button – Turns the fluorescent lamps on or off. Closing the sash automatically turns the lights off. When the lights are in Smart-Start mode, raising the sash turns the lights on automatically.

Outlet Button – Turns the electrical outlets in the work area on or off.


UV Light Button – Turns the UV lamp on or off. When the UV lamp is in Smart-Start mode, closing the sash turns the light on. When the sash is raised, the light turns off automatically.

Timer Button – Allows you to select either a repeating interval timer, or an elapsed timer (stopwatch).

OK/Mute Button – Mutes all audible alarms for approximately 5 minutes, unless there is a system error alarm. When in the Menu mode, this button is used to select an option.

Menu Button – This button toggles the display between the display and menu modes. When in the menu mode, pressing this button returns you to the previous menu level.

Select Buttons – Allow you to choose different options in the menu mode.

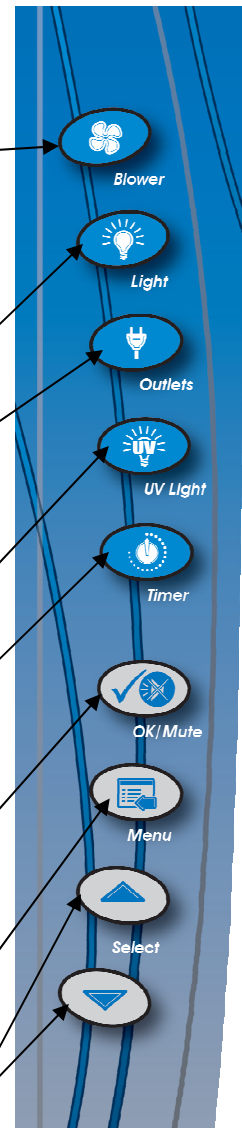

Navigating the Logic+ Menu Screens

MyLogic™ allows you to use the Smart-Start or Night-Smart features that activate functions automatically when the sash is opened or closed.


If equipped, the UV lamp can be programmed to operate for a given time interval when the sash is closed, before it shuts off.

NOTE: When you are in the menu mode, if a selection is not made within 30 seconds, the display will reset back to display mode.

Keypad operations are shown as *blue bold italic*. Menu screen selections are shown as *green italics*.

NOTE: Pressing the appropriate touchpad button will override Smart-Start or Night-Smart selections.

To access the menu, press the *Menu* button. The display panel will show the first level menu. To select from the various menu options press the ▲ or ▼ buttons until the selected option is displayed. Press *OK* to accept that option, or press *Menu* to return to the previous menu level.

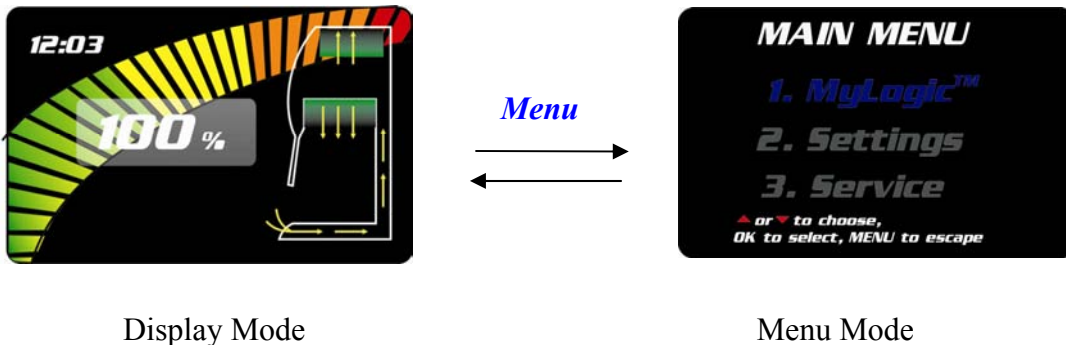

Display Mode


Menu Mode

Navigating the MyLogic™ Menu Screens

The MyLogic screens will allow you to set the cabinet's clock, and to personalize its operation. Please note all MyLogic screens have a blue background.

Setting the Clock

Using the ▲ and ▼ buttons on the touchpad, highlight the *MyLogic* option-it will turn blue when selected. Press **OK** to enter the first MyLogic screen:

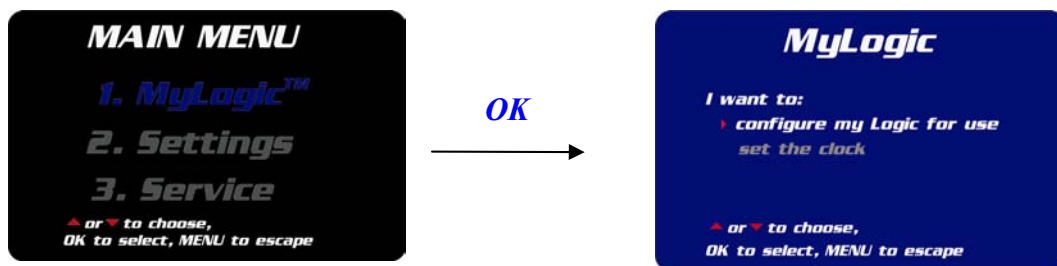

Using the ▲ and ▼ buttons on the touchpad, highlight *set the clock* -it will turn white when selected. Press **OK** to enter the first clock setting screen:

At this screen, select whether you want the clock to display in a 12- or 24-Hour format. When you have highlighted your choice, press **OK** to go to the next screen...



Use the ▲ and ▼ buttons to select the hour, and press **OK**...



Use the ▲ and ▼ buttons to select the minute, and press **OK** to return to the first MyLogic screen.



Configuring the Logic+

In the first MyLogic screen, use the ▲ and ▼ buttons on the touchpad to highlight *configure my Logic for use* -it will turn white when selected. Press **OK** to enter the first configuration screen:

The first screen gives you the option of activating the Smart-Start option for the blower; if you want the cabinet blower to start every time you raise the sash, select *start*, and then press **OK**. If *not start* is selected, then the blower must be manually started from the keypad. When **OK** is pressed, the next configuration screen will appear.

The next screen gives you the option of activating the Smart-Start option for the fluorescent light; if you want the lights to turn on every time you raise the sash, select *turn on*, and then press **OK**. If *stay off* is selected, then the lights must be manually turned on from the keypad. When **OK** is pressed, the next configuration screen will appear.

If you want the cabinet blower to run slowly, maintaining reduced airflows every time you close the sash, select *go into Night-Smart mode* and then press **OK**. If *stop* is selected, then the blower will stop when the sash is closed. When **OK** is pressed, the next configuration screen will appear.

If your Logic+ is configured for a UV light, then you will see the next two screens; if you want the UV lamp to turn on every time you close the sash, select *go into Night-Smart mode*, and then press **OK**. If *stay off* is selected, then the UV light will not turn on when the sash is closed. When **OK** is pressed, the final configuration screen will appear.



If you choose to use Night-Smart option for the UV lamp, this screen allows you to control the time the UV lamp will remain on after the sash is closed. Use the ▲ and ▼ buttons on the touchpad to cycle through the time intervals available, and then press **OK** to select it. The screen will then return to the first MyLogic screen.




Navigating the Settings Menu Screens

The Settings screens will allow an administrator to set some of the cabinet's operational parameters. Please note all Settings screens have a green background.


Units of Measure

Note: The Units of Measure refers to the display of airflow velocities if the cabinet is equipped with the optional airflow sensor.

Using the ▲ and ▼ buttons on the touchpad, highlight the *Settings* option-it will turn green when selected. Press **OK** to enter the first Settings screen:

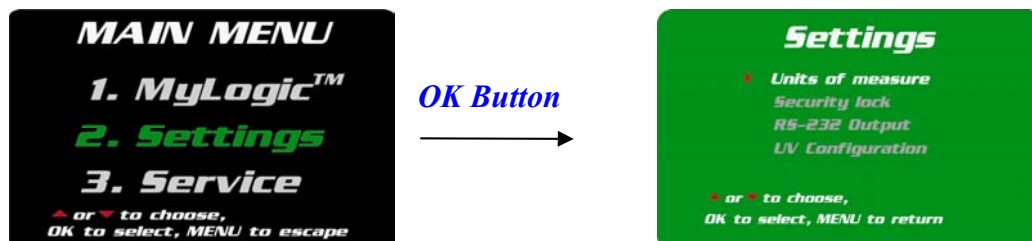


Using the ▲ and ▼ buttons on the touchpad, highlight the *Units of Measure* option-it will turn white when selected, and then press **OK**. Using the ▲ and ▼ buttons on the touchpad, highlight either *metric* or *imperial* units of measure-it will turn white when selected, and then press **OK**. The screen will then return to the first Settings screen.

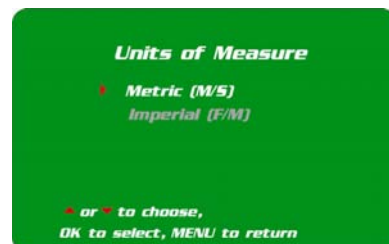

Security Lock

Note: The Security Lock feature “locks” the keypad to prevent unauthorized use of the cabinet. The security lock is unlocked by pressing the ▼ button three times within 2 seconds. The lock reactivates whenever the sash is closed, or the blower shuts off.

From the Settings menu screen, use the ▲ and ▼ buttons on the touchpad to highlight the *Security Lock* option-it will turn white when selected. Press **OK** to enter the Security Lock screen. Using the ▲ and ▼ buttons on the touchpad, highlight either *turned on* or *turned off*-it will turn white when selected, press **OK**. The screen will then return to the first Settings screen.

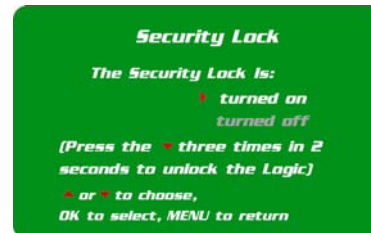


RS-232 Output Rate

Note: This selection will only work if the optional EN/RS-232 board is installed.

This menu option selects the rate that the RS-232 board outputs data. Data can be output at a rate of once per second, once every 10 seconds, once every 30 seconds, or once per minute.

From the Settings menu screen, use the ▲ and ▼ buttons on the touchpad to highlight the *RS-232 output*-it will turn white when selected. Press **OK** to enter the RS-232 output screen. Using the ▲ and ▼ buttons on the touchpad, highlight either the data output rate preferred. It will turn white when selected, and then press **OK**. The screen will then return to the first Settings screen.

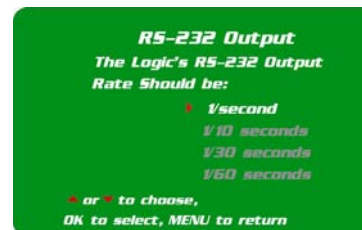

UV Settings

For models equipped with the optional UV light the Logic+ has an integral UV light maintenance system. It allows you to define how many hours you want the UV lamp to operate before receiving a reminder to replace it, a way to monitor how many hours the lamp has been on, and the means to reset the UV lamp hourmeter.

UV Lamp Hourmeter

This display only shows how many hours the UV lamp has been lit, and how many hours remain until you will receive a warning to replace the lamp.

From the Settings menu screen, use the ▲ and ▼ buttons on the touchpad to highlight the *UV Settings* option-it will turn white when selected. Press **OK** to enter the UV Settings screen. Using the ▲ and ▼ buttons on the touchpad, highlight UV Hourmeter-it will turn white when selected, and then press **OK**. The screen will then return to the UV Hourmeter screen.




This screen displays how many hours the UV lamp has operated, and how many hours of operation remain before replacement is recommended. When finished with this screen, press **MENU** to return to the first UV Settings screen.



Reset UV Lamp Hourmeter

This option lets you reset the UV hourmeter to 0 hours whenever the lamp has been replaced.


This screen allows you to reset the UV Hourmeter to 0 hours if you press **OK**. Pressing **MENU** will return you to the first UV Settings screen without resetting the hourmeter.

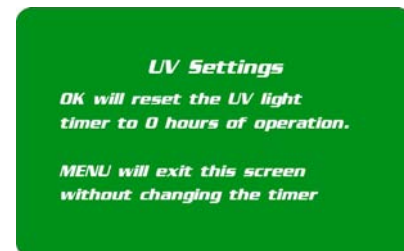

Change UV Lamp Life

In this screen, you can set the number of operating hours before receiving the replace UV lamp warning. For most UV lamps, the output of UV light decreases at a constant rate. Typically, after 6,000 hours of operation the lamp will output 80% of the UV light it did when it was new. This option allows you to set operational life of the UV lamp, in 100 hour increments.

From the UV Settings menu screen, use the ▲ and ▼ buttons on the touchpad to highlight the *Set UV Life* option-it will turn white when selected. Press **OK** to enter the Set UV life screen. Use the ▲ and ▼ buttons to increase or decrease the lamp life in 100 hour increments, until the desired value is displayed, and then press **OK**. The screen will then return to the UV Settings screen.

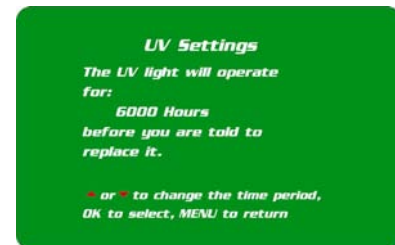

The Service Menu Screens

Note: The Service Menu screens are reserved for use by trained certification personnel as part of the certification or service procedures. All of the screens have a yellow background, and those portions of the Service Menu screens that can alter the performance of the Logic+ are password protected. If you have any questions about these screens, contact Labconco's Product Service Department at 1-800-821-5525 or www.labconco.com for assistance.

Timer Operation

NOTE: The timer button allows activation of an interval (countdown) or stopwatch (elapsed) timer. The timers cannot be operated simultaneously.

To access the main timer menu, press the **Timer** button anytime during normal operation. The main timer menu is shown on the LCD display. Use the **▲** and **▼** buttons to highlight the **Interval** or **Stopwatch** Timer. Press the **OK** button to select the highlighted timer function.

Interval Timer Operation

1. When selected, the Interval Timer menu is displayed on the LCD. The timer defaults to 0:00:00 (hours:minutes:seconds).
2. Press and hold the **▲** or **▼** buttons to increase or decrease the timer interval.
3. When the proper interval is entered on the display, press the **OK** button to start the timer.
4. When the timer reaches 0:00:00, an audible alarm will sound, and the timer will reset itself and repeat the countdown.
5. Press the **OK** button to pause the timer.
6. Press the **Menu** button to clear the interval timer and return to the main timer menu.

Stopwatch Timer Operation

1. When selected, the Stopwatch Timer menu is displayed on the LCD. The timer defaults to 0:00:00.
2. Press the **OK** button to start the timer.
3. Press the **OK** button again to zero the timer.
4. Press the **Menu** button to clear the stopwatch timer and return to the main timer menu.

If An Airflow Alert Activates

The most common causes of an Airflow Alert are:

- Blockage of the inlet grilles or exhaust outlet.
- Removal of the work surface or grille during operation.

Resetting the Airflow Alert System

The Airflow Alert automatically resets to normal operation once the motor speed has stabilized.

Chapter 5: Using The Cabinet

Working In the Biosafety Cabinet


Note: A more thorough review of using the BSC can be found in: *Biosafety in Microbiological and Biomedical Laboratories (BMBL)*, Published by the Centers for Disease Control and Prevention (www.cdc.gov/biosafety/publications).

Planning

- Thoroughly understand procedures and equipment required before beginning work.
- Arrange for minimal disruptions, such as room traffic or entry into the room while the cabinet is in use.

Start-up

- Turn off UV light if included.
- Slowly raise the sash until the bottom of the sash aligns with the sash indicator decal located on the left side of the work area.
- Turn on the fluorescent light and cabinet blower if the Smart-Start features have not been activated.
- Check the air grilles for obstructions.
- Allow the cabinet to operate until the display screen is shown.

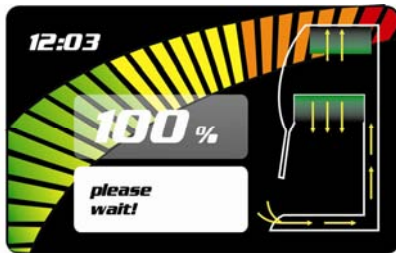

Warming up Screen



Display Screen

- Wash hands and arms thoroughly with germicidal soap.
- Wear appropriate personnel protective equipment (PPE).

Wipe-Down

- Raise the sash to its full open position (approximately 21.75 inches or 552 mm). Mute the alarm by depressing the "OK/Mute" switch.
- Wipe down the interior surfaces of the cabinet with 70% ethanol, or a suitable disinfectant, and allow to dry.

Loading Materials and Equipment

- Only load the materials required for the procedure. Do not overload the cabinet.
- Do not obstruct the front, side, or rear return air grilles.
- Large objects should not be placed close together.
- Slowly close the sash until it is in the correct operating position.
- After loading the cabinet, wait two to three minutes to purge airborne contaminants from the work area.

Work Techniques

- Keep all materials at least 4 inches (100 mm) inside from the sash, and perform all contaminated operations as far to the rear of the work area as possible.
- Segregate all clean and contaminated materials in the work area.
- Arrange materials to minimize the movement of contaminated materials into clean areas.
- Keep all discarded contaminated material to the rear of the work area.
- Avoid moving materials or the operator's hands and arms through the front access opening during use.
- Avoid the use of an open flame. Use disposable labware or an electric incinerator as alternatives.
- Use proper aseptic technique.
- Avoid using techniques or procedures that disrupt the airflow patterns of the cabinet.
- If there is a spill or splatter during use, all objects in the cabinet should be surface decontaminated before removal. Thoroughly disinfect the working area of the cabinet WHILE IT IS STILL IN OPERATION, to prevent the release of contaminants from the cabinet.

Final Purging

- Upon completion of work, the cabinet should be allowed to operate for two to three minutes undisturbed, to purge airborne contaminants from the work area.

Chapter 5: Using The Cabinet

Unloading Materials and Equipment

- Objects in contact with contaminated material should be surface decontaminated before removal from the cabinet.
- All open trays or containers should be covered before being removed from the cabinet.

Wipe-Down

- Wipe down the interior surfaces of the cabinet with a suitable disinfectant, or 70% ethanol, and allow to dry.
- Periodically lift the work surface and wipe down the area beneath it.
- Inspect and clean the towel catch located at the rear of the work area, beneath the work pan.
- Dispose of rubber gloves appropriately, and have lab coat laundered properly.
- Wash hands and arms thoroughly with germicidal soap.

Shutdown

- Lower the sash to turn off the fluorescent light and cabinet blower and activate the UV light if appropriate.

Note: Cell Logic Biosafety Cabinets with Scope-Ready Package will not allow for easy movement of the sash with the microscope eyepieces installed. The blower and safety interlock system will typically work in manual mode for these models unless the microscope is disengaged from the Pure-Vu Seal.

- If appropriate for Cell Logic Biosafety Cabinets with Temp-Zone Package, activate the UV light.

Chapter 6: Maintaining the Cabinet

The common service operations necessary to maintain the biosafety cabinet for peak performance are listed below.

Note: This manual covers operation and maintenance operations for the owners/users of the Logic+ biosafety cabinets. Complete certification procedures, service operations and specifications are published in a separate publication *Technical Manual: Purifier® Logic®+ Biosafety Cabinets*. This manual is available from Labconco's website: www.labconco.com. A complete certifier service kit is available to qualified certifiers from Labconco. Call Labconco's Product Service Department at 800-821-5525 or 816-333-8811.



Do NOT contact blower wheel while still in motion.

NE PAS être en contact avec la roué du ventilateur tant qu'il est en marche.

Routine Maintenance Schedule

Weekly

- Wipe down the interior surfaces of the cabinet with a suitable disinfectant, or 70% ethanol, and allow to dry.
- Using an appropriate glass cleaner, or LabSolutions™ Glass & Surface Wipes, Labconco part # 1570000; clean the sash and the surface of the UV lamp, if so equipped.
- Operate the cabinet blower, noting the percent filter life remaining in an operational log.

Monthly (or more often as required)

- Using a damp cloth, or LabSolutions Glass & Surface Wipes, Labconco part # 1570000; clean the exterior surfaces of the cabinet,

Chapter 6: Maintaining The Cabinet

particularly the front and top of the cabinet, to remove any accumulated dust.

- Disinfect and lift the work surface. Surface disinfect the area beneath the work surface with a suitable disinfectant, or 70% ethanol, and allow to dry. Check the towel catch for retained materials.
- Check all service valves, if so equipped, for proper operation.
- Check the UV and fluorescent light hourmeters, and record their readings in an operational log.
- All weekly activities.

Semiannually or Annually

- Have the cabinet re-certified by a qualified certification technician.
- All monthly activities.

Service Operations

Work Surface Removal:

Note: The work surface must be thoroughly decontaminated before removing it from the cabinet.

Note: The Temp-Zone package option has a prop rod on both sides to aid in pivoting and cleaning. The Temp-Zone work surface requires disconnection of the tubing from the quick connect fittings on the left side of the cabinet before removal.

1. Lift the front edge of the work surface straight up by grasping the knob handles at either front corner.
2. Pull the work surface straight out, letting its rear edge rest on the center support underneath.
3. Reinstall the work surface by resting the bottom on the center rail while pushing it back into the cabinet. Be sure to engage the tabs on the back corners of the work surface with the slots on the rear wall of the work area.

Front Grille Removal:

Note: The grille must be thoroughly decontaminated before removing it.

1. Remove the work surface as described earlier.
2. At one end of the grille, grip the front of grille with one hand, and the back with the other hand. Pivot that end of the grille upward and inward, paralleling the angle of the sash, as shown in Figure 6-1.
3. Pull the other end of the grille up and away from the bottom edge of the cabinet.
4. Reinstall the grille by reversing the above sequence, ensuring that the grille properly engages the bottom edge of the cabinet.

Figure 6-1



Chapter 6: Maintaining The Cabinet


Towel Catch Removal:

Although not normally required, the towel catch can be removed for cleaning, inspection, etc.

Note: The work surface of the cabinet and the towel catch must be thoroughly decontaminated before removing either.


1. Remove the work surface as described above.
2. Remove the towel catch by pivoting the bottom out toward you, as shown in Figure 6-2; it is spring loaded, and you will feel some resistance. Note the orientation of the towel catch.
3. Surface decontaminate the towel catch before removing it.
4. Reinstall the towel catch by sliding it back into position, in the correct orientation. Also ensure that the Sampling/Decontamination Tube (the black tube with an orange cap) rests behind the towel catch, allowing the catch to contact the rear wall of the cabinet.

Figure 6-2

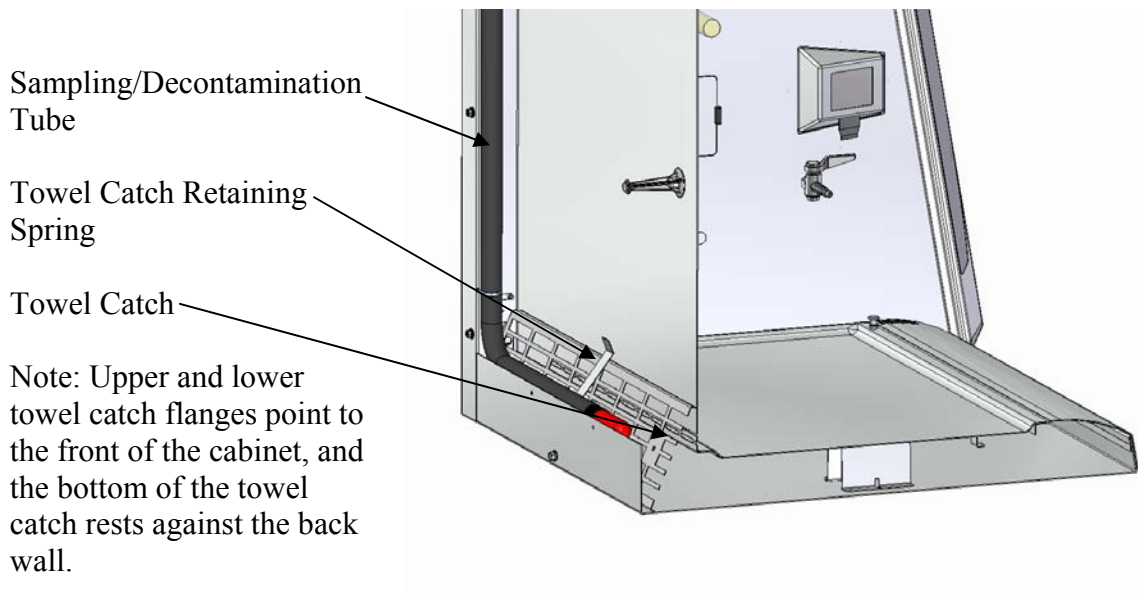

Font Panel Removal and Installation:**Figure 6-3**

1. Locate and remove the two Phillips screws that secure the front panel as shown in Figure 6-3. They are located on the bottom corners of the front dress panel.
2. Swing the bottom of the dress panel out to clear the fluorescent light and then lift the front dress panel straight up and away from the cabinet.

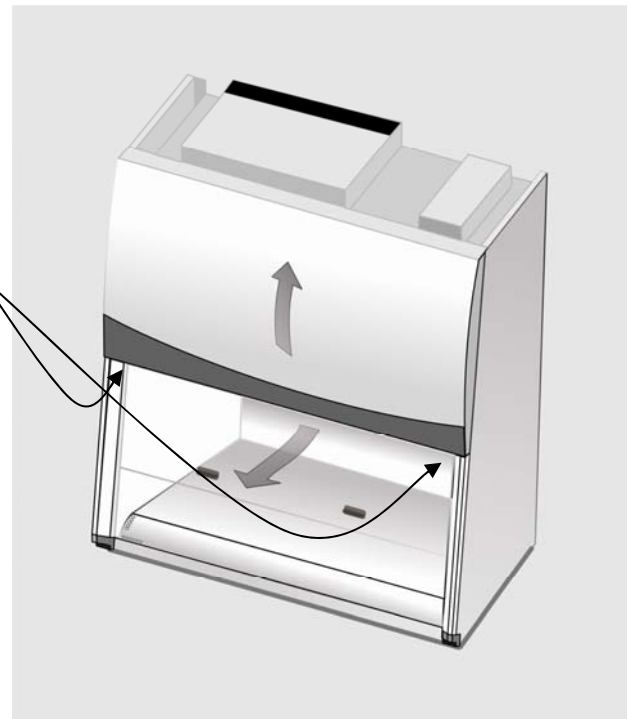**Figure 6-4**

1. To reinstall the panel, reverse these steps, ensuring that the plastic pin in the top corners of the dress panel properly engage the corner posts.



Chapter 6: Maintaining The Cabinet

Changing the Fluorescent Lamps:

1. Unplug the cabinet or turn off the System Reset Switch located on the top of the cabinet.
2. Remove the front dress panel as noted in Figure 6-3.
3. Remove the fluorescent lamps by pulling the lamp sockets straight off each end of the lamp, and releasing both lamps from the spring clips that secure them in place.
4. Install the new lamps by reversing the removal procedure.

Changing the Optional UV Lamp:

Note: For optimum performance, the UV lamp should be changed on an annual basis, or as indicated by the UV lamp timer.

The UV lamp and the work area of the cabinet must be thoroughly decontaminated before removing the lamp.


1. Start the cabinet and let it operate for 5 minutes.
2. Raise the sash to its full open position.
3. Thoroughly surface decontaminate the UV lamp and the work area of the cabinet.
4. Unplug the cabinet or turn off the System Reset Switch, located on the top of the cabinet.
5. Remove the UV lamp by rotating it 90 degrees and lifting it straight up and out of its sockets.
6. Install new lamp by reversing the removal procedure.

Resetting a Circuit Breaker:

To reset any of the circuit breakers located on the left side of the electronics module, depress the white button until it sets.

Figure 6-5

Circuit Breakers- The front breaker protects the electrical outlets, the rear breaker protects the motor and lights.

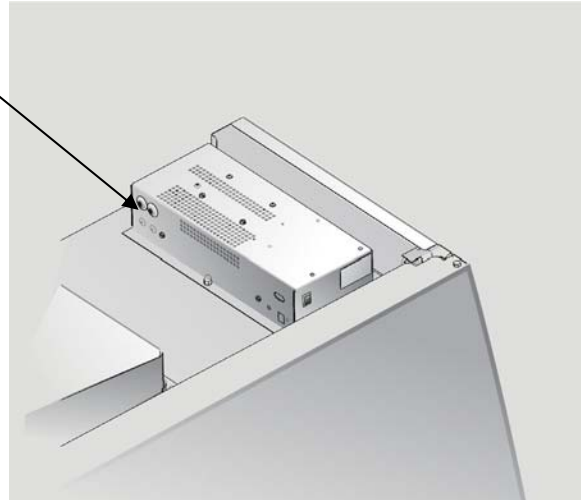**Storage**

If the biosafety cabinet is to be left unused for more than one month, it should be prepared for storage.

Note: The cabinet should not be stored in areas of excess humidity or temperature extremes. If the cabinet is moved during storage, it must be recertified before use.

1. Close the sash completely and seal the bottom edge and the exhaust outlet with plastic sheeting.
2. Unplug the cabinet.
3. Ensure that the cabinet will not be moved or disturbed while being stored.

Chapter 7: Troubleshooting

Refer to the following table if the biosafety cabinet fails to operate properly. If the suggested corrective actions do not solve the problem, contact Labconco for additional assistance.

PROBLEM	CAUSE	CORRECTIVE ACTION
Cabinet blower and lights won't turn on	Unit not plugged into outlet	Plug the biosafety cabinet into appropriate electrical service. Check connection to control box on top of cabinet.
	System Reset Switch is Off	Turn on the System Reset Switch.
	Circuit breaker(s) tripped	Reset circuit breakers.
	Keypad disconnected or defective	Run keypad diagnostics and check connections.
Blower won't turn on	Sash closed	Raise sash.
	Keypad disconnected or defective	Run keypad diagnostics and check connections.
	Blower wiring is disconnected	Inspect blower wiring.
	Blower motor is defective	Replace blower motor.

PROBLEM	CAUSE	CORRECTIVE ACTION
Fluorescent light not working	Sash is closed	Open sash – Fluorescent lights will not work with the sash closed.
	Lamp(s) are defective	Replace defective lamp(s)
	Lamp wiring is disconnected	Inspect lamp wiring.
	Defective lamp ballasts	Replace lamp ballasts.
Fluorescent light is dim or flickering	Keypad disconnected or defective	Run keypad diagnostics and check connections.
	Lamp(s) are defective	Replace defective lamp(s)
	Lamp wiring is disconnected	Inspect lamp wiring.
UV light not working	Defective lamp ballast	Replace lamp ballast.
	Sash is open	Close sash – UV light will not work with the sash open.
	Lamp is defective	Replace defective lamp.
	Lamp wiring is disconnected	Inspect lamp wiring.
UV light is dim or flickering	Defective lamp ballast	Replace lamp ballast.
	Keypad disconnected or defective	Run keypad diagnostics and check connections.
	Lamp is defective or is at end of operating lifetime.	Replace defective or worn out lamp.
UV light is dim or flickering	Lamp wiring is disconnected	Inspect lamp wiring.
	Defective lamp ballast	Replace lamp ballast.

Chapter 7: Troubleshooting

PROBLEM	CAUSE	CORRECTIVE ACTION
Airflow Alert goes off and/or there is a slight decrease in filter life remaining gauge	HEPA filter loading	The gauge reading steadily decreases as the cabinet is used.
	Blockage of the return air slots or grille	Check all return air slots and grilles to ensure that they are not blocked or restricted.
	Blockage of the exhaust outlet	Ensure that the exhaust outlet is not blocked or restricted.
Contamination of work in the cabinet	Blockage or restriction under the work surface	Ensure that the towel catch and plenum beneath the work surface are unobstructed.
	Improper technique or procedure for the biosafety cabinet	See “Use of the cabinet” section in the manual.
	Restriction of the return air slots or grille – blockage of the exhaust outlet	Ensure that all return air slots, grilles and the exhaust outlet are unobstructed.
	External factors are disrupting the cabinet airflow patterns or acting as a source of contamination	See “Working in the Biosafety Cabinet” section of this manual.
	Cabinet is out of adjustment/HEPA filter(s) are defective	Have cabinet recertified.

Appendix A: Components


Illustration A-1 indicates the location of the following service parts, and replacement accessory parts:

Biosafety Cabinet Replacement Parts

Item	Quantity	Part No.	Description
1	1	3838500	Exhaust HEPA Filter 3-ft
1A	1	3838501	Exhaust HEPA Filter 4-ft
1B	1	3838502	Exhaust HEPA Filter 5-ft
1C	1	3838503	Exhaust HEPA Filter 6-ft
2	1	3838400	Supply HEPA Filter 3-ft
2A	1	3838401	Supply HEPA Filter 4-ft
2B	1	3838402	Supply HEPA Filter 5-ft
2C	1	3838403	Supply HEPA Filter 6-ft
3	2	9721901	Lamp, Fluorescent, 3-ft
3A	2	9721900	Lamp, Fluorescent, 4-ft
3B	2	9721903	Lamp, Fluorescent, 5- & 6-ft
4	1	1271300	Lamp, UV (models with UV light only)
5	14	1885404	Screw, #6-32 x 0.25" PH (for Pure-Vu Seal – not shown, see Figure 3-5)


Appendix A: Components

A-1


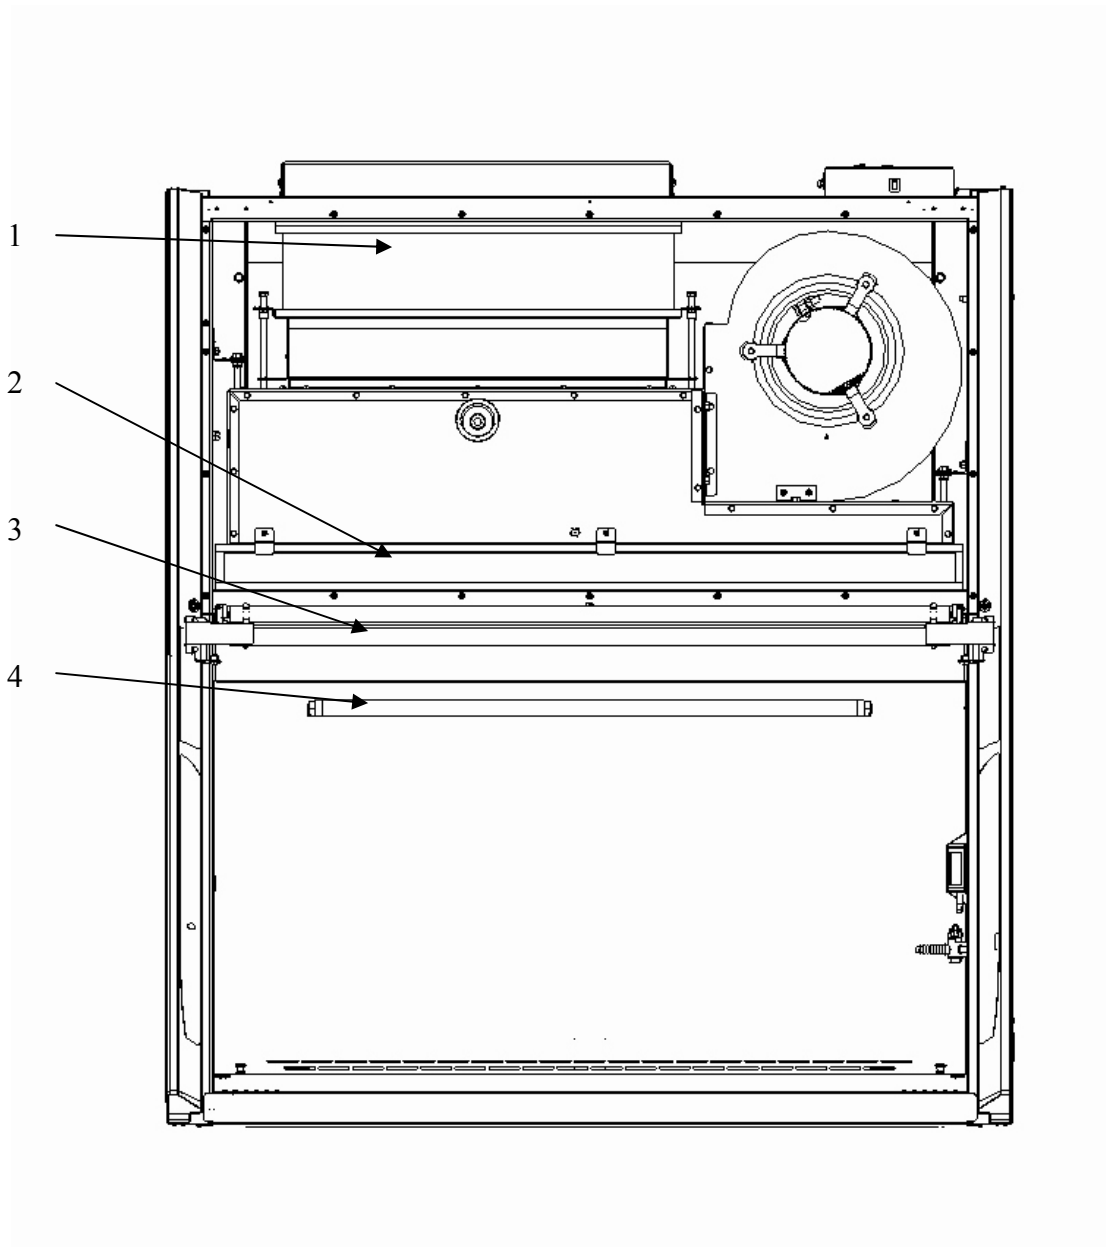


Appendix B: Dimensions

B-1

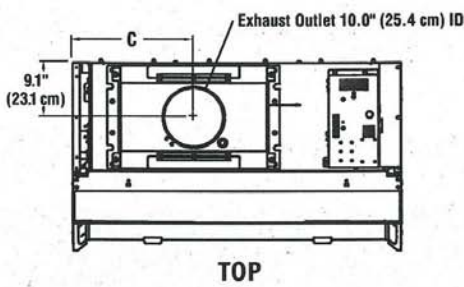

Nominal Width	A Inches/cm	B Inches/cm	C Inches/cm
3'	42.3/107.4	36.5/92.7	13.6/34.5
4'	54.3/137.9	48.5/123.2	19.9/50.5
5'	66.3/168.4	60.5/153.7	26.9/68.3
6'	78.3/198.9	72.5/184.2	32.9/83.6

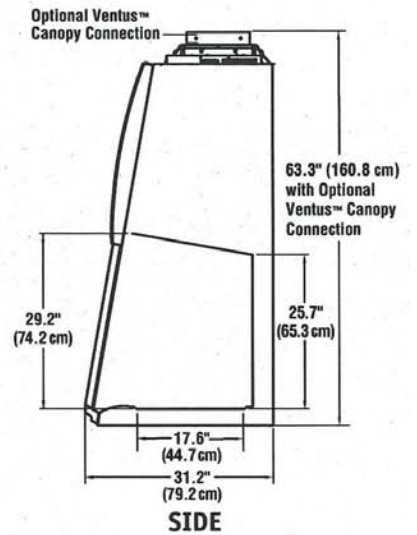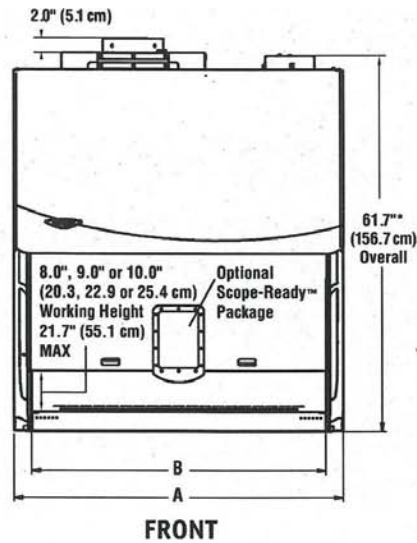

Appendix C: Specifications

Electrical Data

Model #	Requirements
3X23xxx0x	115 VAC, 60 Hz, 12 Amps
3X23xxx1x	100 VAC, 50/60 Hz, 12 Amps
3X23xxx-20, 30, 40, 50, 60, 70	230 VAC, 50/60 Hz, 6 Amps
3X24xxx0x	115 VAC, 60 Hz, 12 Amps
3X24xxx1x	100 VAC, 50/60 Hz, 12 Amps
3X24xxx-20, 30, 40, 50, 60, 70	230 VAC, 50/60 Hz, 6 Amps
3X25xxx0x	115 VAC, 60 Hz, 16 Amps
3X25xxx1x	100 VAC, 50/60 Hz, 16 Amps
3X25xxx-20, 30, 40, 50, 60, 70	230 VAC, 50/60 Hz, 8 Amps
3X26xxx0x	115 VAC, 60 Hz, 16 Amps
3X26xxx1x	100 VAC, 50/60 Hz, 16 Amps
3X26xxx-20, 30, 40, 50, 60, 70	230 VAC, 50/60 Hz, 8 Amps

Motor Specifications

Cabinet Model	Electrical Requirements
All 3- and 4-foot Cabinets, all Voltages	1/2 H.P. Electronically Commutated Motor (ECM) 120-277 VAC – 50/60 Hz, Full Torque – 42 Oz.-Ft (3.56 N-M) 7.7 Full Load Amps @115VAC 4.3 Full Load Amps @230VAC Automatic Thermal Protection

Cabinet Model	Electrical Requirements
All 5- and 6-foot Cabinets, all Voltages	3/4 H.P. Electronically Commutated Motor 120-277 VAC – 50/60 Hz, Full Torque – 66 Oz.-Ft (5.59 N-M) 9.6 Full Load Amps @115VAC 6.8 Full Load Amps @230VAC Automatic Thermal Protection

Environmental Conditions

- Indoor use only.
- Ambient temperature range: 41° to 104°F (5° to 40°C).
- Maximum relative humidity: 80% for temperatures up to 88°F (31°C), decreasing linearly to 50% relative humidity at 104°F (40°C).
- Main supply voltage fluctuations not to exceed $\pm 10\%$ of the nominal voltage.
- Transient overvoltages according to Installation Categories II (Overvoltage Categories per IEC 1010). Temporary voltage spikes on the AC input line that may be as high as 1500V for 115V models and 2500V for 230V models are allowed.
- Used in an environment of Pollution degrees 2 (i.e., where normally only non-conductive atmospheres are present). Occasionally, however, a temporary conductivity caused by condensation must be expected, in accordance with IEC 664.

Appendix D: Accessories

Labconco offers a full line of accessories to enhance your Cell Logic+'s operation and usability. For a complete list of these accessories, please consult our website at www.labconco.com.

Appendix E: Quick Chart

Model	3x239_	3x249_	3x259_	3x269_
Type	A2	A2	A2	A2
Cabinet Size (in feet)	3	4	5	6
Sash Opening (inches)	9	9	9	9
Starting Serial # ¹	1303_	1303_	1303_	1303_
Nominal Avg. Downflow (FPM)	55+/-5	55+/-5	55+/-5	55+/-5
Nominal Average Inflow (FPM)	105+/-5	105+/-5	105+/-5	105+/-5
Supply HEPA Data				
Labconco P/N	3838400	3838401	3838402	3838403
Exhaust HEPA Data				
Labconco P/N	3838500	3838501	3838502	3838503
Motor/Blower Data				
Labconco P/N ²	3832200	3832201	3832208	3832208
Motor HP	1/2	1/2	3/4	3/4
Fluorescent/UV Lamp Data				
Fluorescent Lamps (2 each)	F25T8 TL741	F32T8 TL741	F40T8 SP41	F40T8 SP41
UV Lamp	G30T8	G30T8	G30T8	G30T8

1. The primary serial tag is on the lower outside edge of the right corner post. The secondary serial tag is located on the front of the electronics module on the top right side of the cabinet. The first two digits of the serial number are the year of production; the next two are the month. The next 5 digits are the sequence of production, and the letter following the serial number is the revision level of the cabinet.
2. Each motor must be programmed by Labconco for the appropriate width cabinet.

Appendix F: Installation Guide for all Pure-Vu Seals and Stand-Still Isolation Platforms

Figure F-1 is an aid to show the proper installation of the pure-Vu Seal for the Cell Logic Biosafety Cabinet with Scope-Ready Package. Figure F-1 also shows the proper placement of the Stand-Still Isolation Platform.



Figure F-1

Appendix F: Installation Guide Pure-Vu Seals/Stand-Still Isolation Platforms

Figure F-2 is an aid to show the Pure-Vu Seal fully installed with the eyepieces extended and sealed. Figure F-2 also shows the microscope moved forward into proper position on the Stand-Still Isolation Platform.



Figure F-2

Appendix F: Installation Guide Pure-Vu Seals/Stand-Still Isolation Platforms

Stereoscopes with forward extending bases and frequent eyepiece height adjustment typically require the selection of a Pure-Vu XL Seal and Stand-Still XL Isolation Platform. Figures F-3 through F-10 are an aid in setting up the pleated Pure-Vu XL Seal. Figures F-11 and F-12 show typical complete installations of stereo microscopes and proper placement of the Stand-Still XL Isolation Platform. Listed next are instructions for setting up the pleated design of the Pure-Vu XL Seal.

1. Per Figure F-3, with the outer aerodynamic collar removed, place the Pure-Vu XL Seal over the inner aerodynamic mounting collar. Locate the top five holes and secure with transparent tape as shown. Pure-Vu XL Seals allow for eyepiece height flexibility of +/- 2.0" (51 mm).



Figure F-3

2. Per Figure F-4, form the first pleat and secure with transparent tape. The seal shown has pre-cut eyepiece holes (Labconco #4027811) and is designed for the upper portion of the glass cutout. This upper portion of the glass cutout is used frequently with stereoscopes. However, should you need a pleat at the middle or lower position of the glass cutout, then the pleat can be moved lower when setting up the Blank Pure-Vu XL Seal (4027810). See Figure F-4.

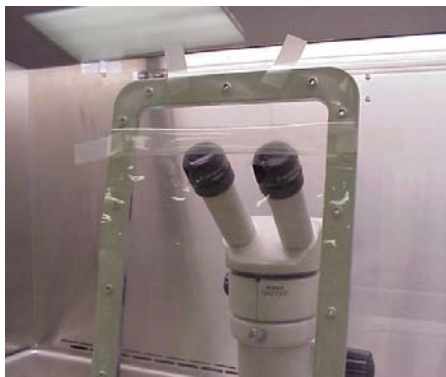


Figure F-4

Appendix F: Installation Guide Pure-Vu Seals/Stand-Still Isolation Platforms

3. Per Figure F-5, form the second pleat and secure with transparent tape.



Figure F-5

4. Per Figure F-6 and Figure 3-5, place the Outer Aerodynamic collar over the Pure-Vu XL Seal and lightly secure in place with the 14 Phillips mounting screws. Do not tighten.



Figure F-6

5. Per Figure F-7, remove the transparent tape and then tighten the 14 Phillips mounting screws.



Figure F-7

Appendix F: Installation Guide Pure-Vu Seals/Stand-Still Isolation Platforms

6. Per Figure F-8, move the microscope forward through the holes in the Pure-Vu Seal and install the eyepiece. A tight seal should be formed around the eyepiece.



Figure F-8

7. Figure F-9 shows the finished installation.



Figure F-9

8. Per Figure F-10, adjust the scope eyepiece height for proper focus for the specimen range.



Figure F-10

Appendix F: Installation Guide Pure-Vu Seals/Stand-Still Isolation Platforms

9. Figure F-11 shows the completed installation of the Pure-Vu XL Seal and Stand-Still XL Isolation Platform for one scope manufacturer. The Pure-Vu XL Seals extend 5.5" below the aerodynamic collar.



Figure F-11

Appendix F: Installation Guide Pure-Vu Seals/Stand-Still Isolation Platforms

10. Figure F-12 shows a different installation of the Pure-Vu XL Seal and Stand Still XL Isolation Platform for another separate scope manufacturer.

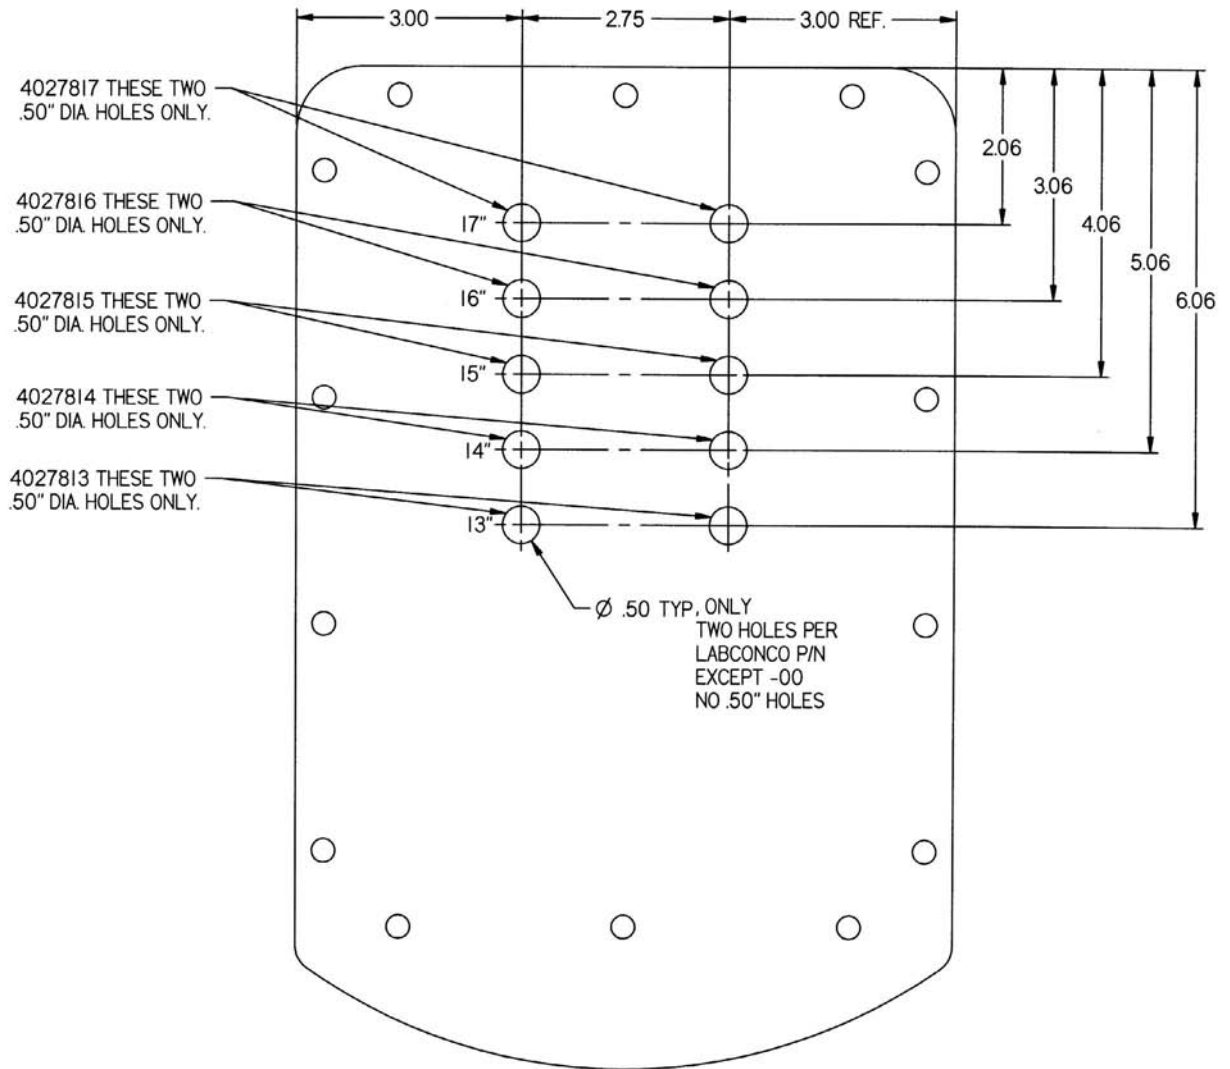


Figure F-12


11. Refer to *Appendix D: Accessories* to order Pure-Vu Seals and Stand Still Isolation Platforms and use *Chapter 3* and *Appendix F* as an aid for proper setup.

Pure-Vu Template

Note: Not to scale, see next page.



Appendix F: Installation Guide Pure-Vu Seals/Stand-Still Isolation Platforms

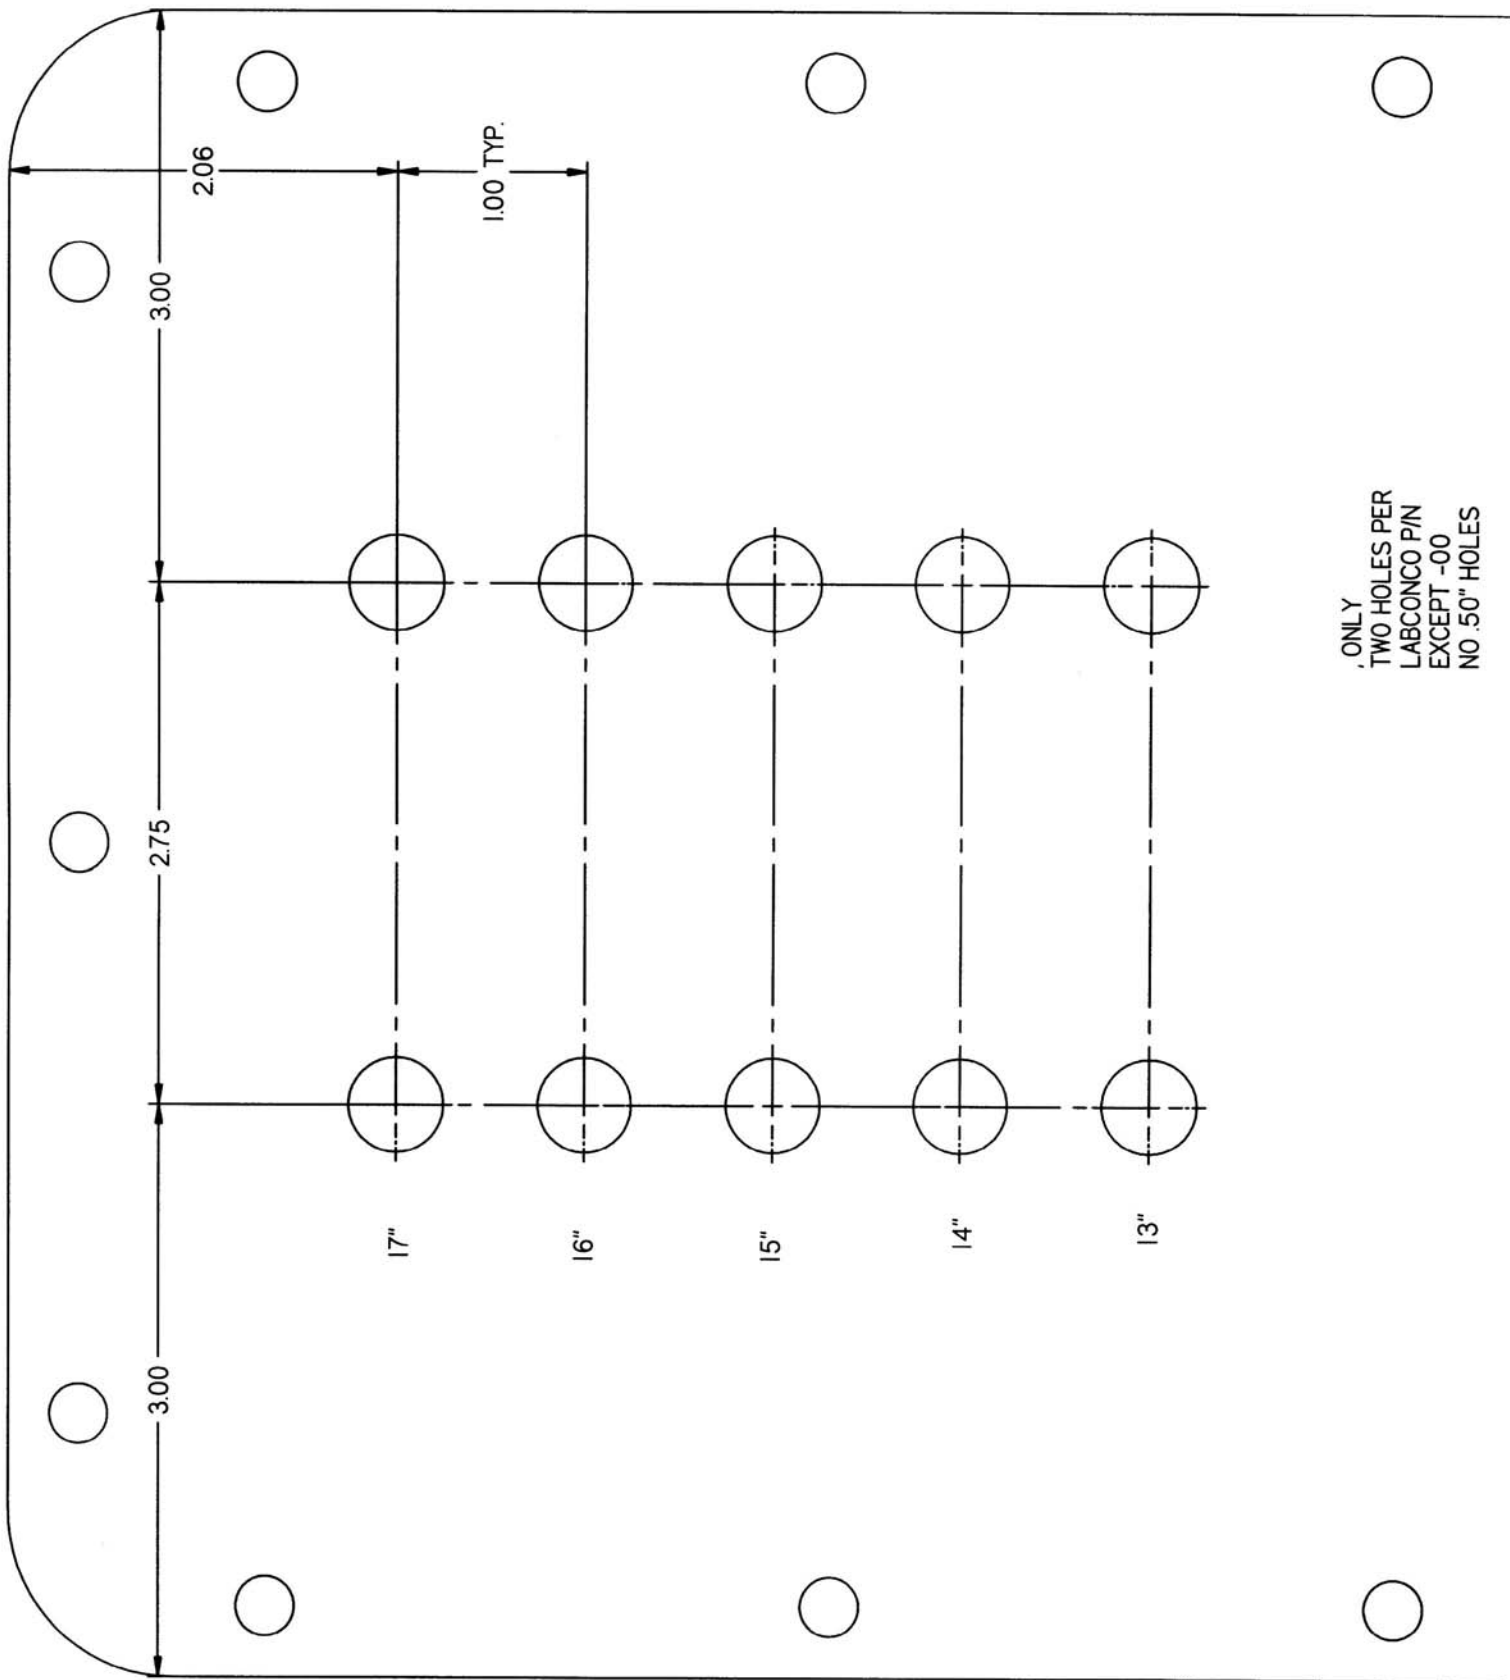

ONLY
TWO HOLES PER
LABCONCO P/N
EXCEPT -00
NO .50" HOLES



Protecting your laboratory environment

LABCONCO

LABCONCO CORPORATION
8811 Prospect Avenue
Kansas City, MO 64132-2696

(816) 333-8811 • (800) 821-5525
FAX: (816) 363-0130
www.labconco.com

CE Declaration of Conformity

We: Labconco Corporation
8811 Prospect Avenue
Kansas City, MO 64132 USA
Ph. 816-333-8811 Fax. 816-363-0130
labconco@labconco.com

being the representative party in the EU solely responsible for this certification, hereby declare that the following product:

Equipment: Laboratory Equipment – Purifier Logic+ Series Biological Safety Cabinets

Type, Model:	32239xx-20, 30, 40, 50, 60, 70	Type A2 3' Wide, 9" Sash
	33239xx-20, 30, 40, 50, 60, 70	Type A2 3' Wide, 9" Sash
	34239xx-20, 30, 40, 50, 60, 70	Type A2 3' Wide, 9" Sash
	32249xx-20, 30, 40, 50, 60, 70	Type A2 4' Wide, 9" Sash
	33249xx-20, 30, 40, 50, 60, 70	Type A2 4' Wide, 9" Sash
	34249xx-20, 30, 40, 50, 60, 70	Type A2 4' Wide, 9" Sash
	32259xx-20, 30, 40, 50, 60, 70	Type A2 5' Wide, 9" Sash
	33259xx-20, 30, 40, 50, 60, 70	Type A2 5' Wide, 9" Sash
	34259xx-20, 30, 40, 50, 60, 70	Type A2 5' Wide, 9" Sash
	32269xx-20, 30, 40, 50, 60, 70	Type A2 6' Wide, 9" Sash
	33269xx-20, 30, 40, 50, 60, 70	Type A2 6' Wide, 9" Sash
	34269xx-20, 30, 40, 50, 60, 70	Type A2 6' Wide, 9" Sash
	32348xx-20, 30, 40, 50, 60, 70	Type B2 4' Wide, 8" Sash
	33348xx-20, 30, 40, 50, 60, 70	Type B2 4' Wide, 8" Sash
	34348xx-20, 30, 40, 50, 60, 70	Type B2 4' Wide, 8" Sash
	32368xx-20, 30, 40, 50, 60, 70	Type B2 6' Wide, 8" Sash
	33368xx-20, 30, 40, 50, 60, 70	Type B2 6' Wide, 8" Sash
	34368xx-20, 30, 40, 50, 60, 70	Type B2 6' Wide, 8" Sash

Manufacturer: Labconco Corporation
8811 Prospect Avenue
Kansas City, MO 64132 USA
Ph. 816-333-8811 Fax. 816-363-0130
labconco@labconco.com

is in conformity with the standards listed below:

EN61010-1
EN61326-1
EN55022
EN61000-3-2/3

following the provisions of the following directives:

89/336/EEC
2004/108/EC
2006/95/EC

when installed and operated in accordance with the manufacturers installation and operating instructions.

Mark Schmitz Kansas City U.S.A. Feb. 28, 2013
Place and date of issue

Mark Schmitz
Vice President, Research and Engineering
Labconco Corporation

Labconco P/N 3696088, Rev. -, ECO H446